

Sample Name :Melittin,honey bee
 Cat No.: RP20415
 Lot No.: E8178020L
 Time Processed :13:44:01
 Month-Day-Year Processed :12/24/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010509

<Chromatogram>

mV

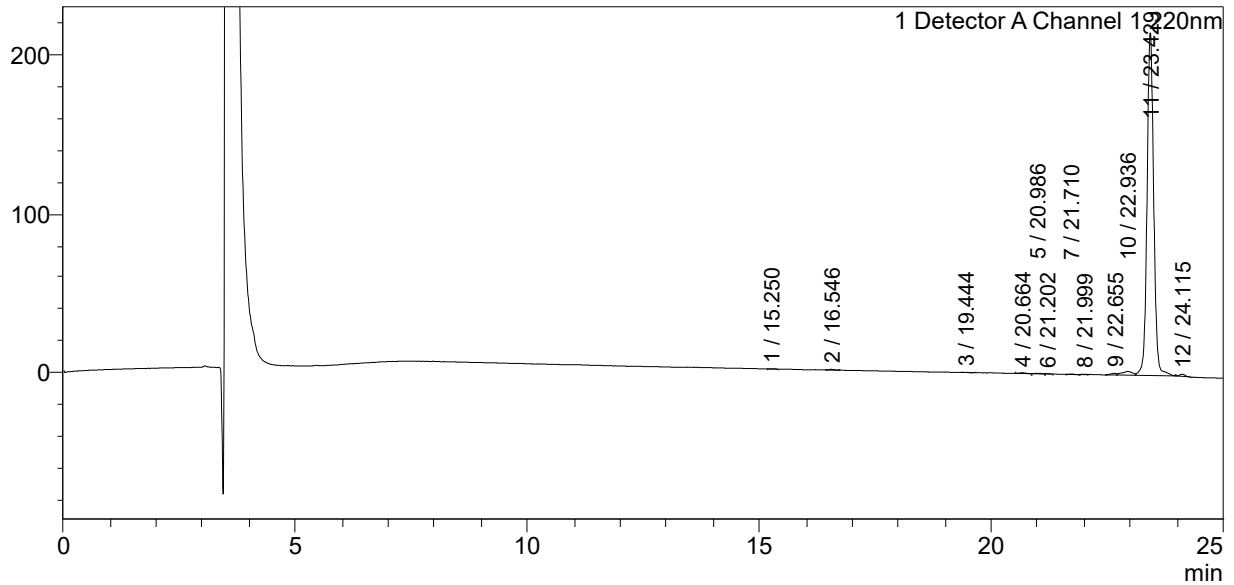

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.250	1096	128	0.049
2	16.546	4269	511	0.191
3	19.444	1638	215	0.073
4	20.664	5454	537	0.244
5	20.986	3471	329	0.155
6	21.202	1383	214	0.062
7	21.710	2042	260	0.091
8	21.999	1946	256	0.087
9	22.655	10094	1073	0.452
10	22.936	38416	2358	1.720
11	23.429	2152494	216475	96.375
12	24.115	11158	1419	0.500
Total		2233461	223774	100.000