


Mass Spectrum

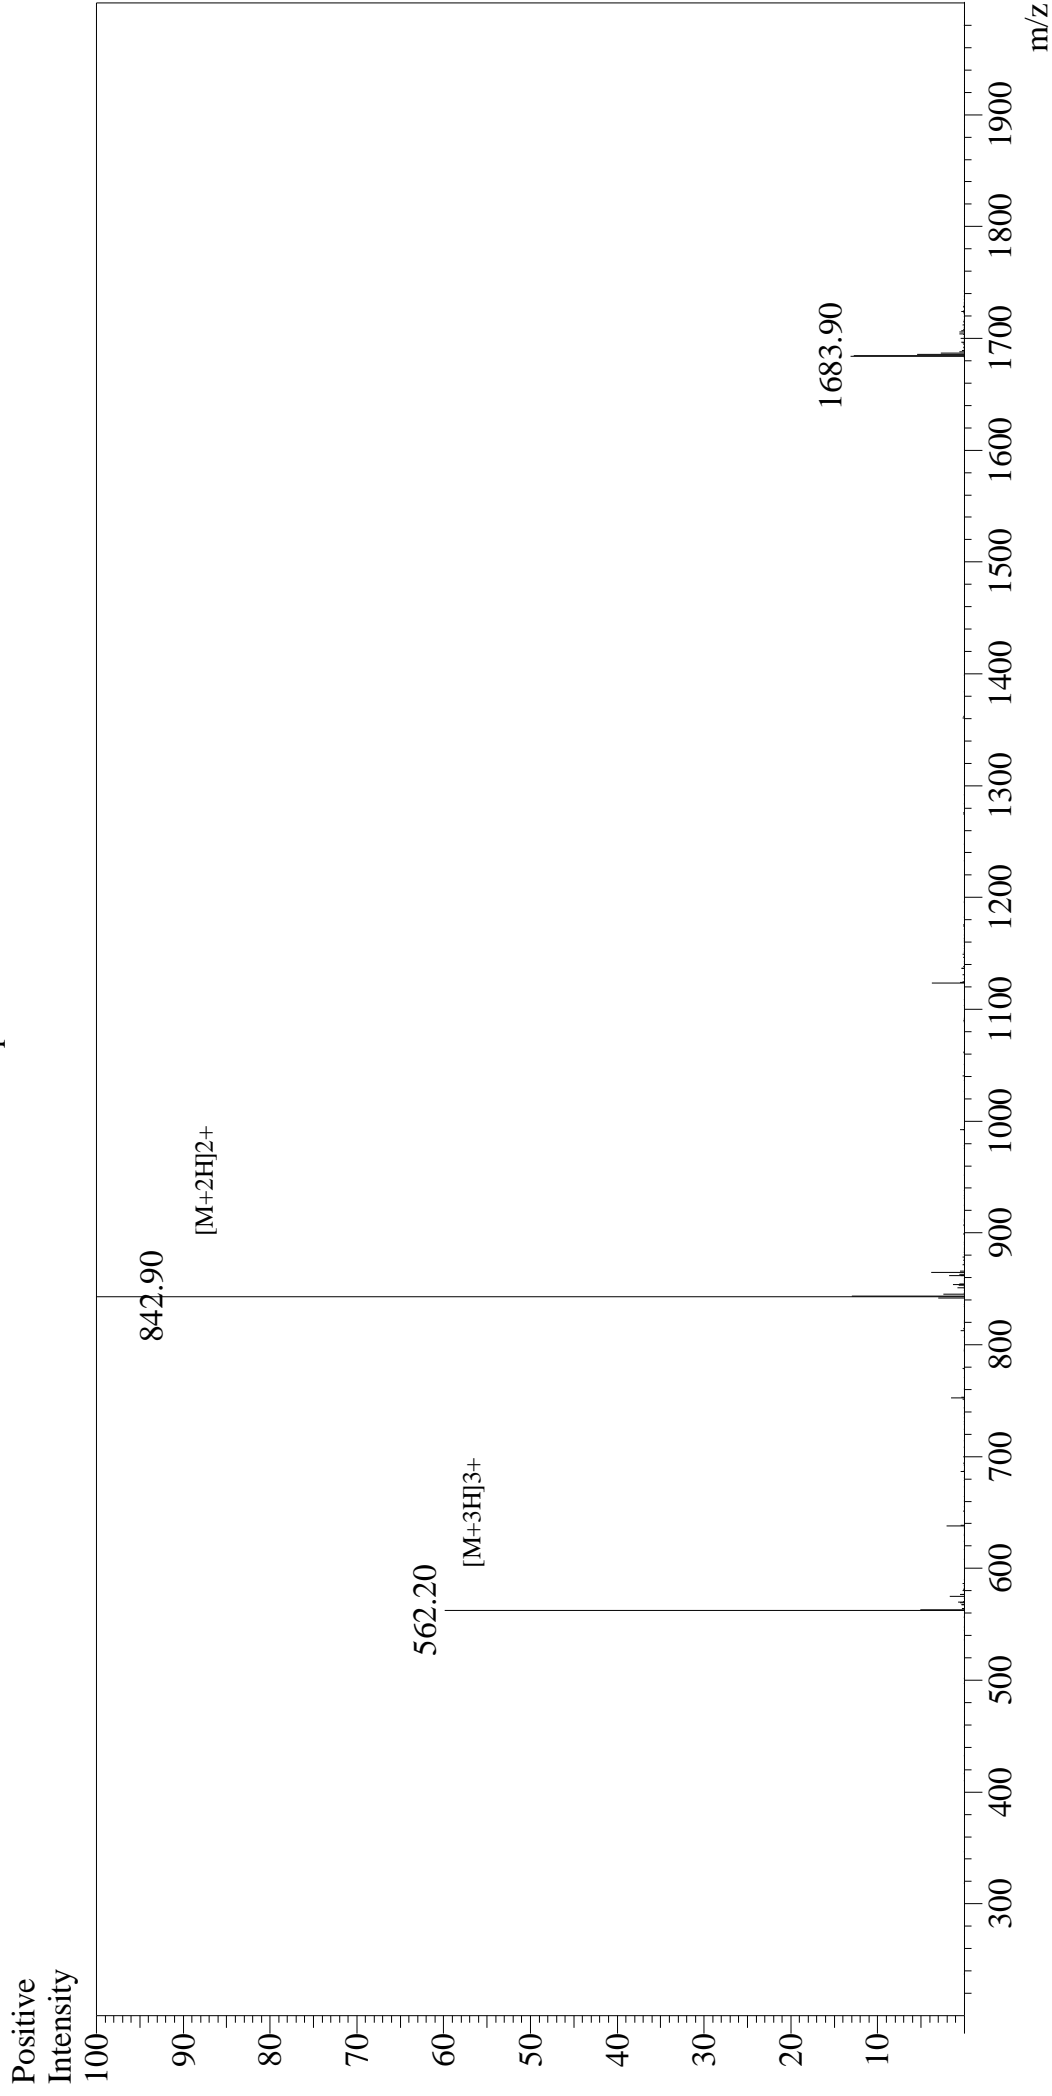

Sample Information

User : Gary
Month-Day Processed : 11/21/16
Time Processed : 14:08:20
Injection Volume : 0.2
Sample Name : α -Factor Mating Pheromone, yeast
Cat No. : RP01002
Lot No. : PE1621611
Theoretical MW : 1683.98
Observed MW : 1683.80

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH