

Sample Name:PACAP (1-38), human, ovine, rat
 Cat No:RP10335
 Lot No :E4917320K
 Time Processed :8:07:26 PM
 Month-Day-Year Processed :11/26/2020


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	15
35.00	Pumps	Pump A B.Conc	15
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

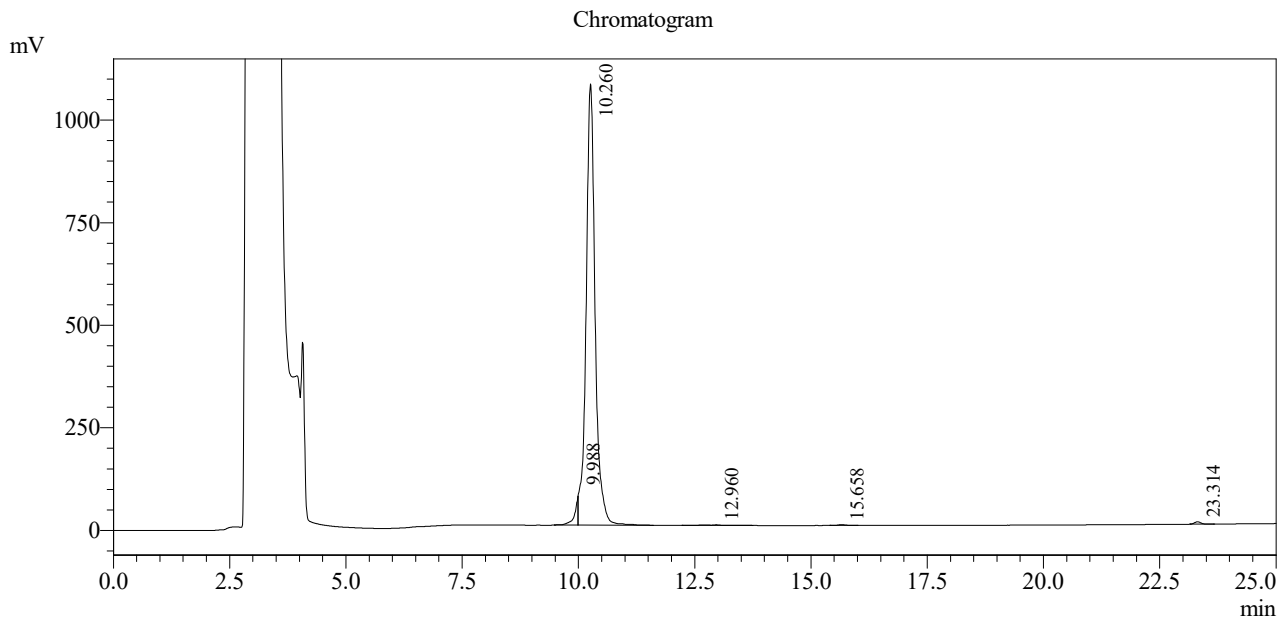

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.988	355035	65057	2.374
2	10.260	14480070	1075277	96.809
3	12.960	46552	1576	0.311
4	15.658	22195	1962	0.148
5	23.314	53530	5727	0.358
Total		14957383	1149598	100.000