

Sample Name: α -Melanocyte-Stimulating Hormone (MSH), amide
 Cat No: RP10644
 Lot No : E4285020L
 Time Processed : 4:41:16 PM
 Month-Day-Year Processed : 01/03/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Module	Command	Value
0.10	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

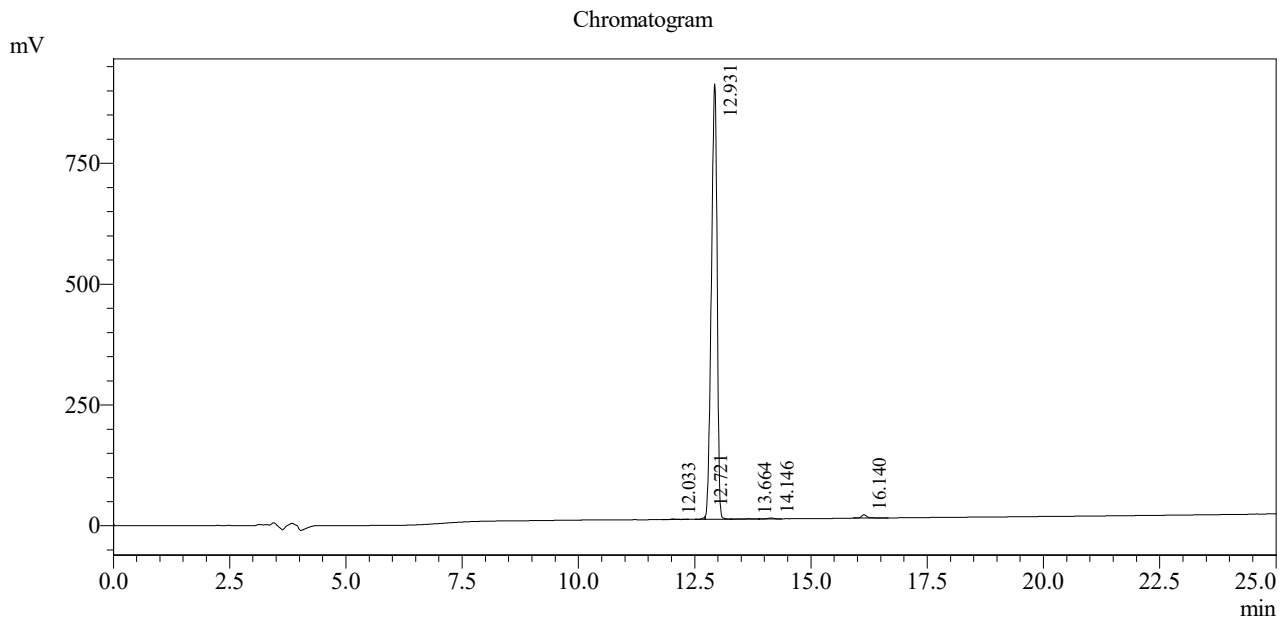

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.033	5817	969	0.074
2	12.721	15973	4245	0.204
3	12.931	7723419	900935	98.688
4	13.664	11840	732	0.151
5	14.146	15481	1838	0.198
6	16.140	53538	6836	0.684
Total		7826066	915555	100.000