

Sample Name :Gastric Inhibitory Peptide (GIP), human  
 Cat No.: RP10795  
 Lot No.: E9514220B  
 Time Processed :13:36:12  
 Month-Day-Year Processed :02/24/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

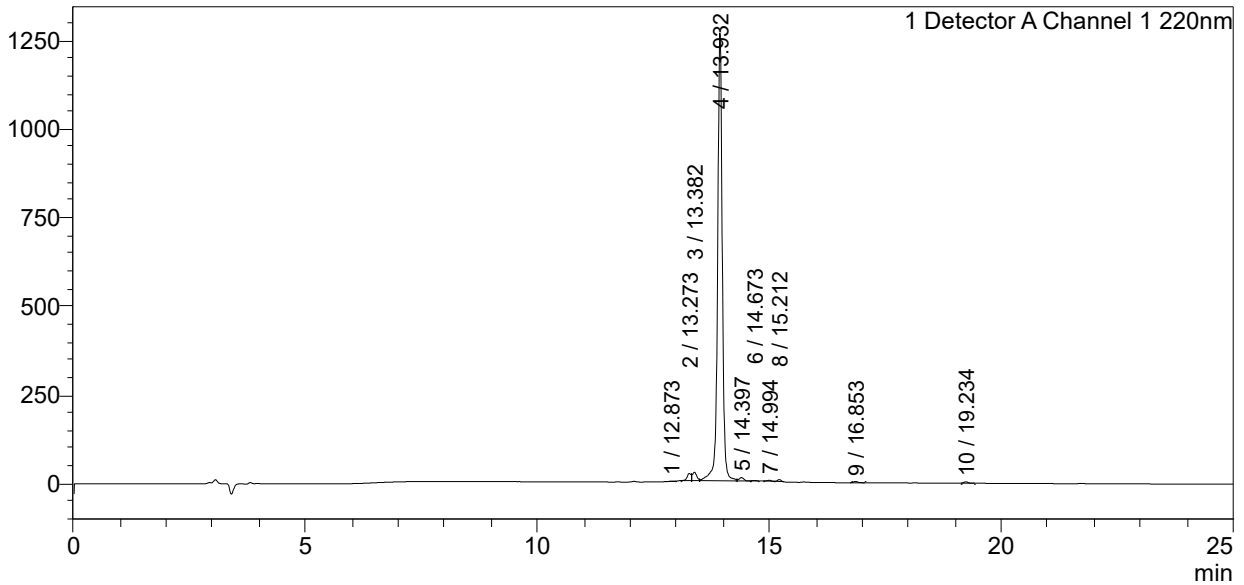

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.873	1855	550	0.020
2	13.273	125951	20412	1.343
3	13.382	157286	23483	1.677
4	13.932	8933330	1262167	95.273
5	14.397	66611	9221	0.710
6	14.673	5508	986	0.059
7	14.994	13570	2511	0.145
8	15.212	27676	5343	0.295
9	16.853	22727	3660	0.242
10	19.234	22067	3628	0.235
Total		9376582	1331961	100.000