

Sample Name : RGD
 Cat. No. : RP20297
 Lot. No. : PE2031702

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

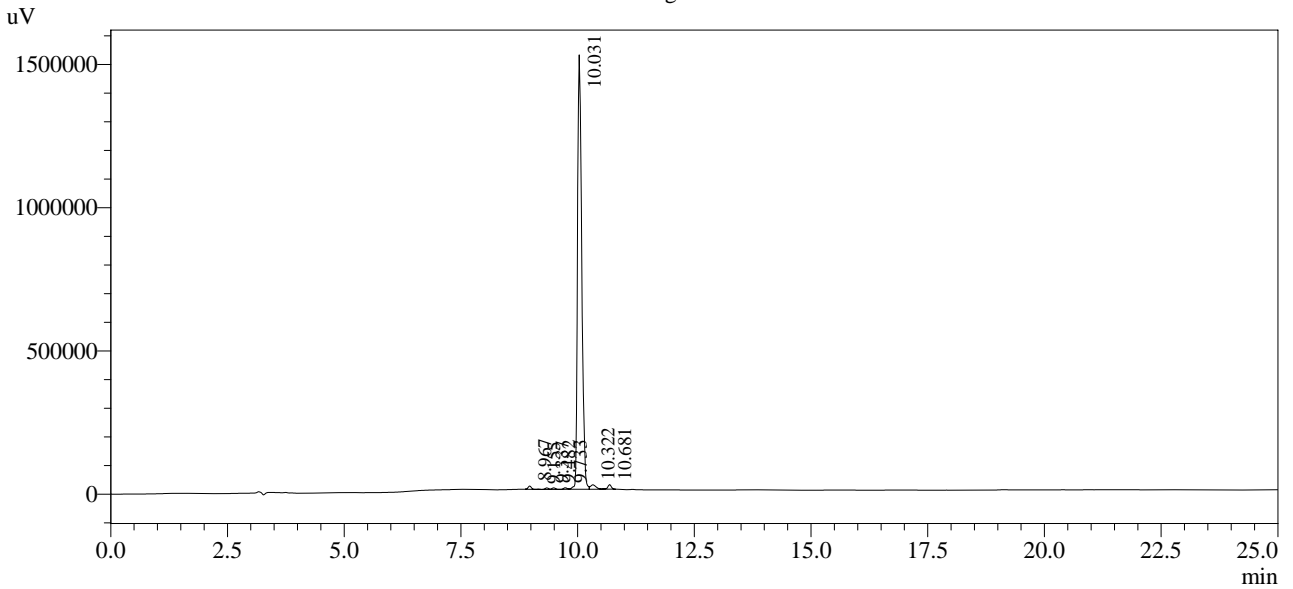

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.967	53662	11093	0.541
2	9.155	3549	811	0.036
3	9.337	27844	5304	0.281
4	9.482	29173	5476	0.294
5	9.733	30089	5201	0.304
6	10.031	9557043	1516384	96.416
7	10.322	124838	15357	1.259
8	10.681	86075	15596	0.868
Total		9912272	1575223	100.000