

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide
 Cat No :RP21087
 Lot No :E4648820J
 Time Processed :21:30:46
 Month-Day-Year Processed :11/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

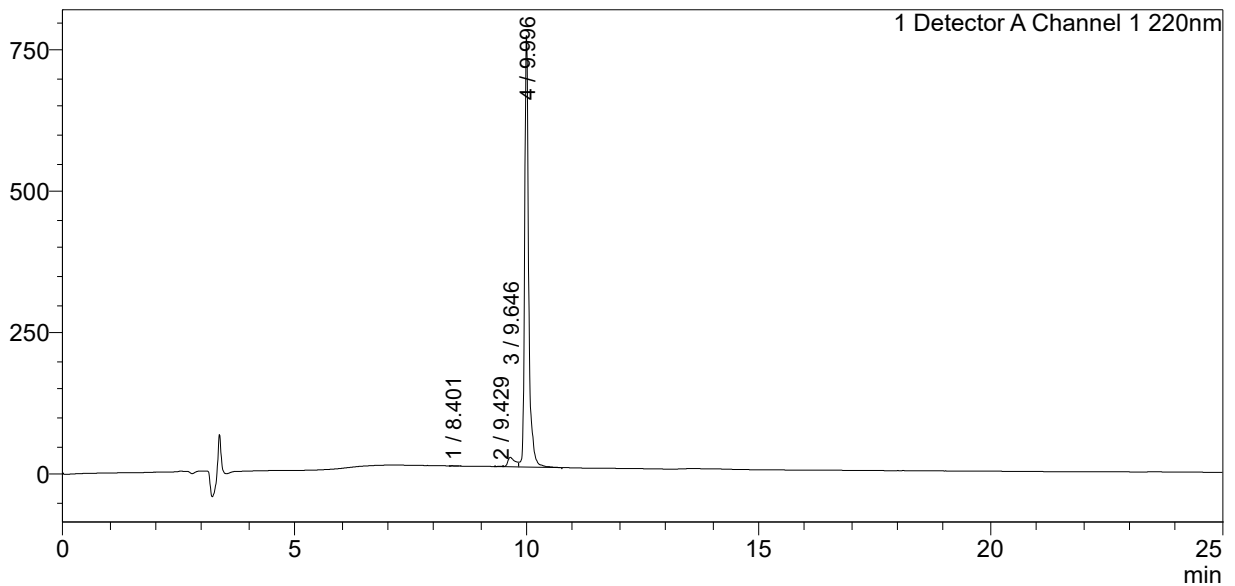

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.401	1414	309	0.030
2	9.429	4296	590	0.090
3	9.646	190828	16879	4.003
4	9.996	4570402	763027	95.877
Total		4766940	780804	100.000