

Sample Name :RGD  
 Cat. No. : RP20297  
 Lot. No. :PE8901902  
 Time Processed :9:49:38  
 Month-Day-Year Processed :03/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

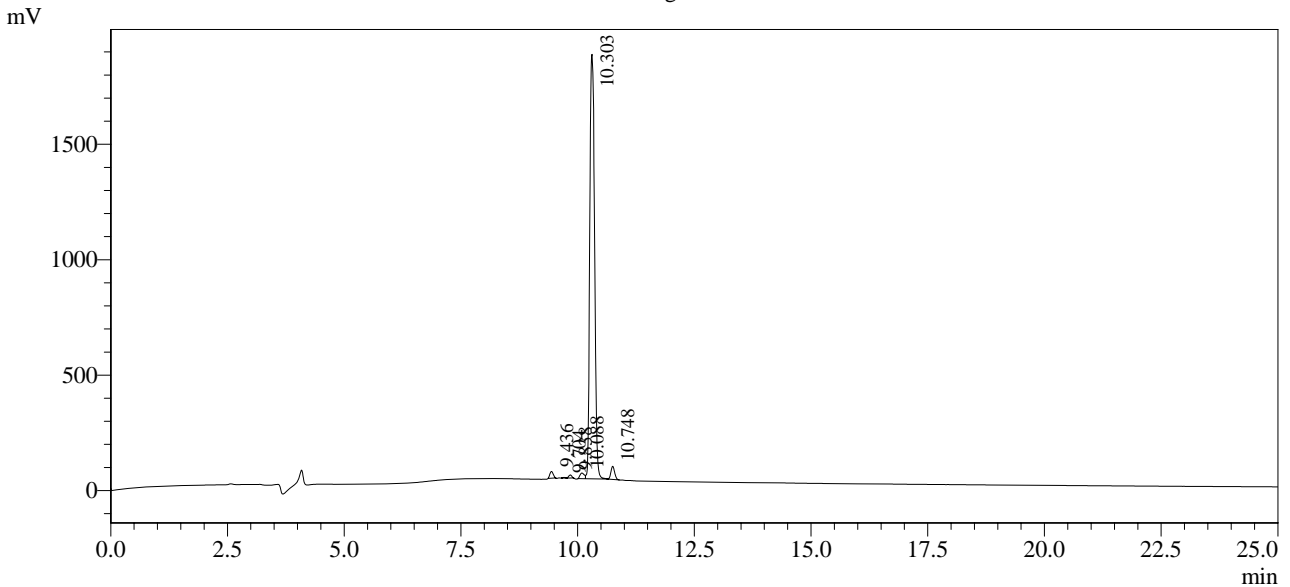

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.436	145011	29299	1.051
2	9.704	10515	2994	0.076
3	9.838	57958	13329	0.420
4	10.088	156400	24334	1.133
5	10.303	13115929	1838914	95.057
6	10.748	312199	56975	2.263
Total		13798011	1965846	100.000