

Sample Name :Angiotensin II, human
 Cat. No. : RP20257
 Lot. No. :E7276319H
 Time Processed :9:01:13
 Month-Day-Year Processed :08/31/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

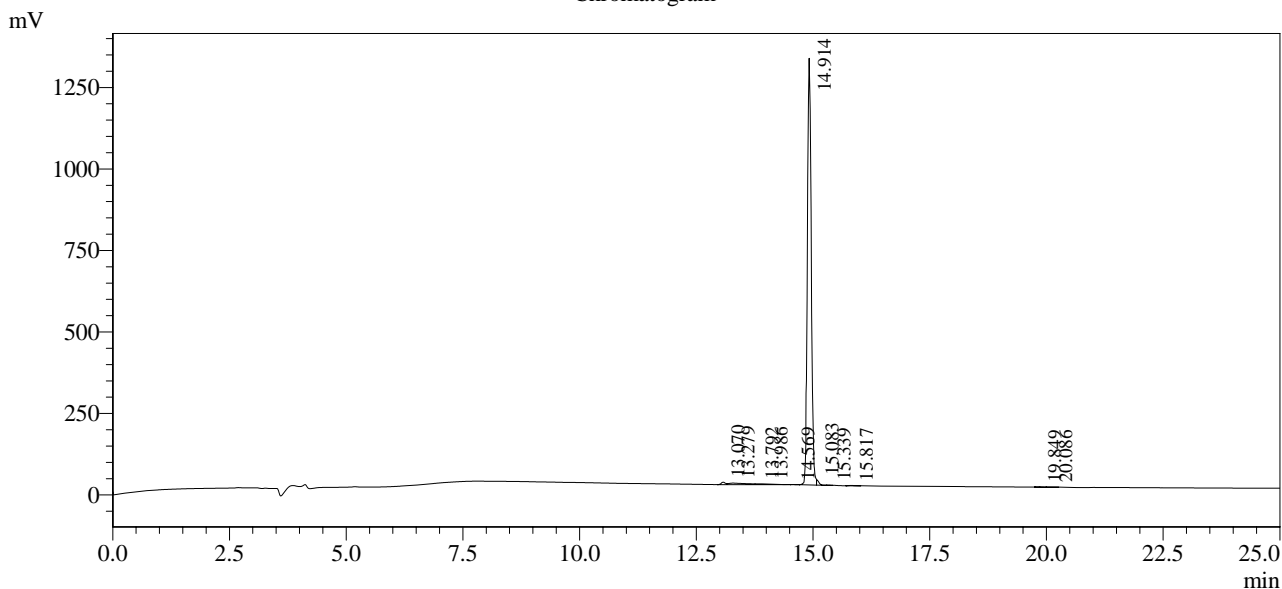

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.070	45968	7507	0.580
2	13.279	123433	4627	1.558
3	13.792	21472	2350	0.271
4	13.986	31844	2165	0.402
5	14.569	1688	278	0.021
6	14.914	7626753	1308970	96.292
7	15.083	50496	16248	0.638
8	15.339	1796	521	0.023
9	15.817	9093	1257	0.115
10	19.849	2867	473	0.036
11	20.086	4999	742	0.063
Total		7920410	1345137	100.000