

Sample Name :IRBP (1-20), human
 Cat. No. : RP20269
 Lot. No. :PE6521706

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
10.00	Pumps	Pump B Conc.	35	
35.00	Pumps	Pump B Conc.	95	
41.00	Pumps	Pump B Conc.	95	
41.01	Pumps	Pump B Conc.	5	
50.00	Pumps	Pump B Conc.	5	
50.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

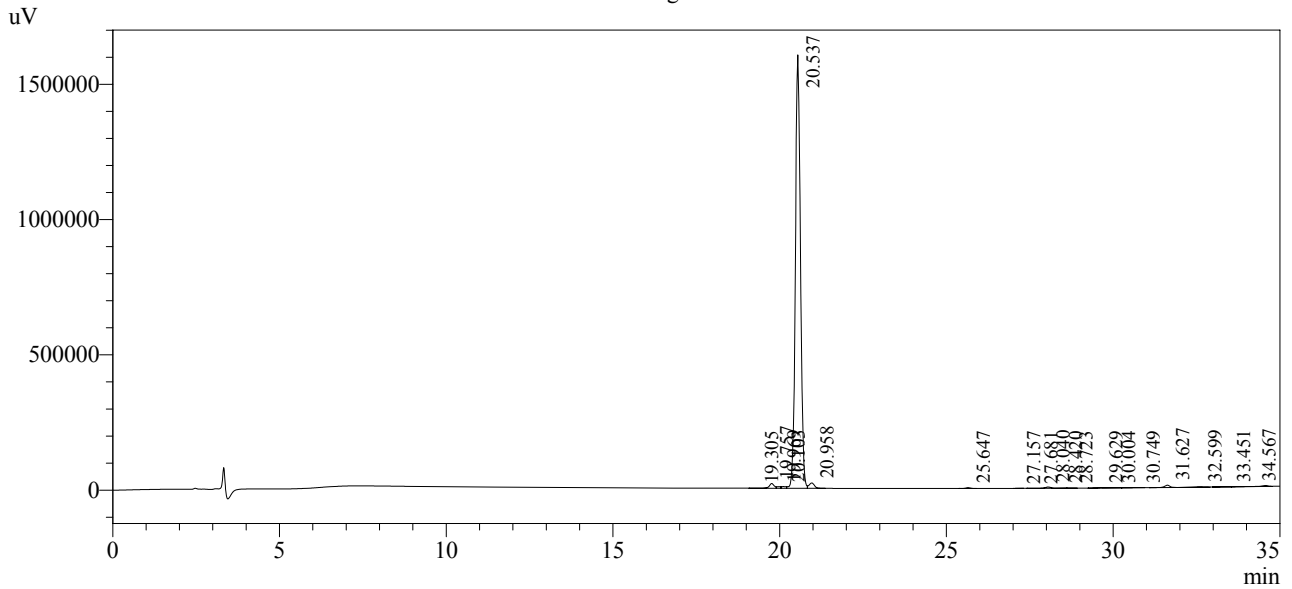

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	19.305	12056	1016	0.068
2	19.757	185097	17754	1.045
3	19.969	46737	6114	0.264
4	20.103	63410	6365	0.358
5	20.537	16901534	1602037	95.400
6	20.958	217036	19694	1.225
7	25.647	26475	2891	0.149
8	27.157	1531	173	0.009
9	27.681	5167	367	0.029
10	28.040	55833	4595	0.315
11	28.420	5100	321	0.029
12	28.723	1617	118	0.009
13	29.629	13383	1078	0.076
14	30.004	8604	575	0.049
15	30.749	5123	170	0.029
16	31.627	96854	8677	0.547
17	32.599	23953	1505	0.135
18	33.451	5219	244	0.029
19	34.567	41786	2994	0.236
Total		17716516	1676688	100.000