

Sample Name :c-Myc Peptide  
 Cat No :RP11731  
 Lot No :E7990420L  
 Time Processed :2:17:08  
 Month-Day-Year Processed :12/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: SS-CM-0309

<Chromatogram>

mV

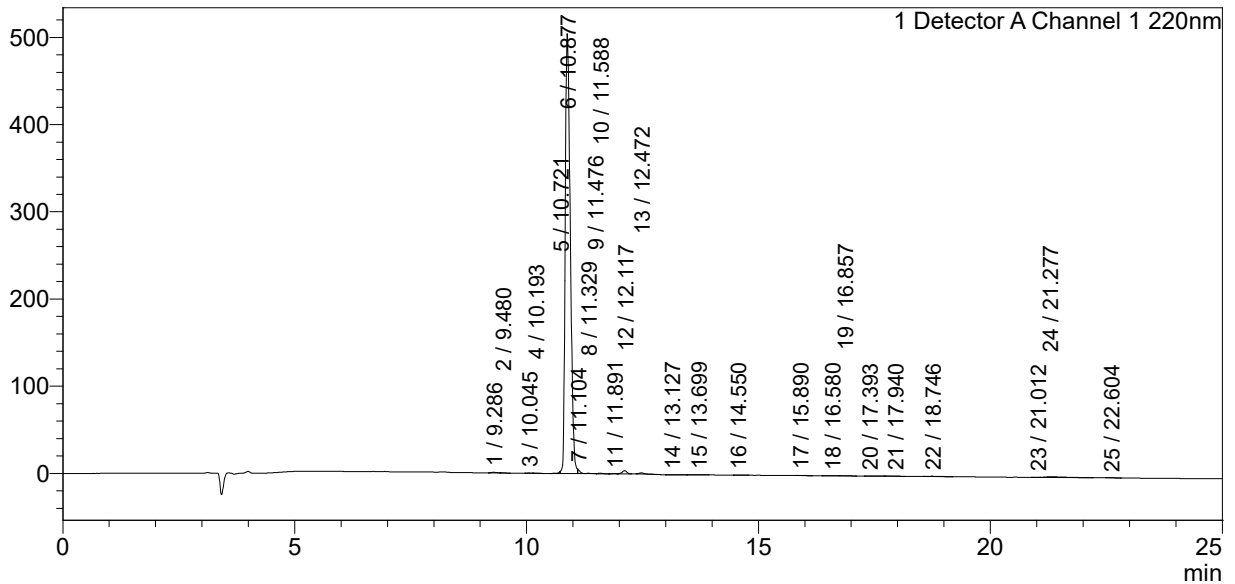

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.286	5952	782	0.151
2	9.480	1981	336	0.050
3	10.045	1151	248	0.029
4	10.193	1030	193	0.026
5	10.721	7599	2137	0.192
6	10.877	3821631	504630	96.691
7	11.104	14925	5163	0.378
8	11.329	2497	444	0.063
9	11.476	1297	276	0.033
10	11.588	4074	609	0.103
11	11.891	1433	235	0.036
12	12.117	25047	3691	0.634
13	12.472	14013	1497	0.355
14	13.127	1291	86	0.033
15	13.699	1983	146	0.050
16	14.550	1689	153	0.043

Peak#	Ret. Time	Area	Height	Area%
17	15.890	1050	94	0.027
18	16.580	1721	160	0.044
19	16.857	1542	114	0.039
20	17.393	2434	191	0.062
21	17.940	3069	226	0.078
22	18.746	6657	401	0.168
23	21.012	1214	154	0.031
24	21.277	24829	804	0.628
25	22.604	2293	279	0.058
Total		3952404	523051	100.000