

Sample Name : Amylin, human, amide  
 Cat No : RP11278  
 Lot No E8002020L  
 Time Processed : 4:24:09 PM  
 Month-Day-Year Processed : 12/26/2020


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010017

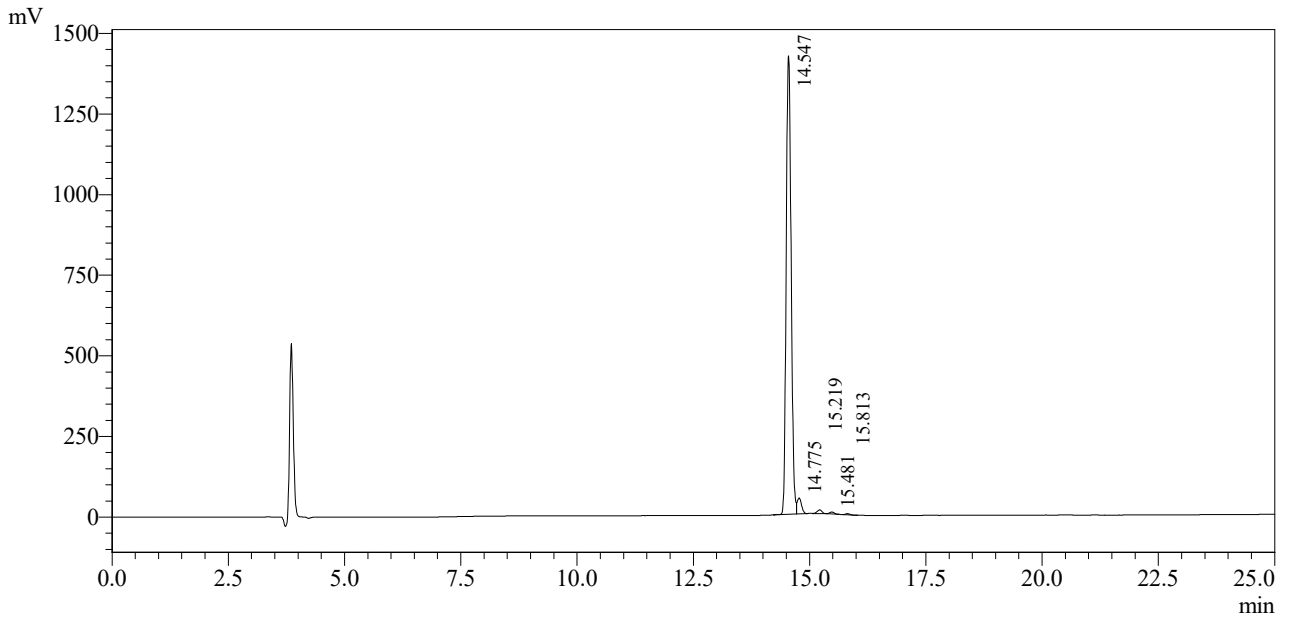

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.547	10473376	1421305	95.853
2	14.775	317417	49512	2.905
3	15.219	79449	11369	0.727
4	15.481	38182	5797	0.349
5	15.813	18034	3461	0.165
Total		10926457	1491445	100.000