


Mass Spectrum

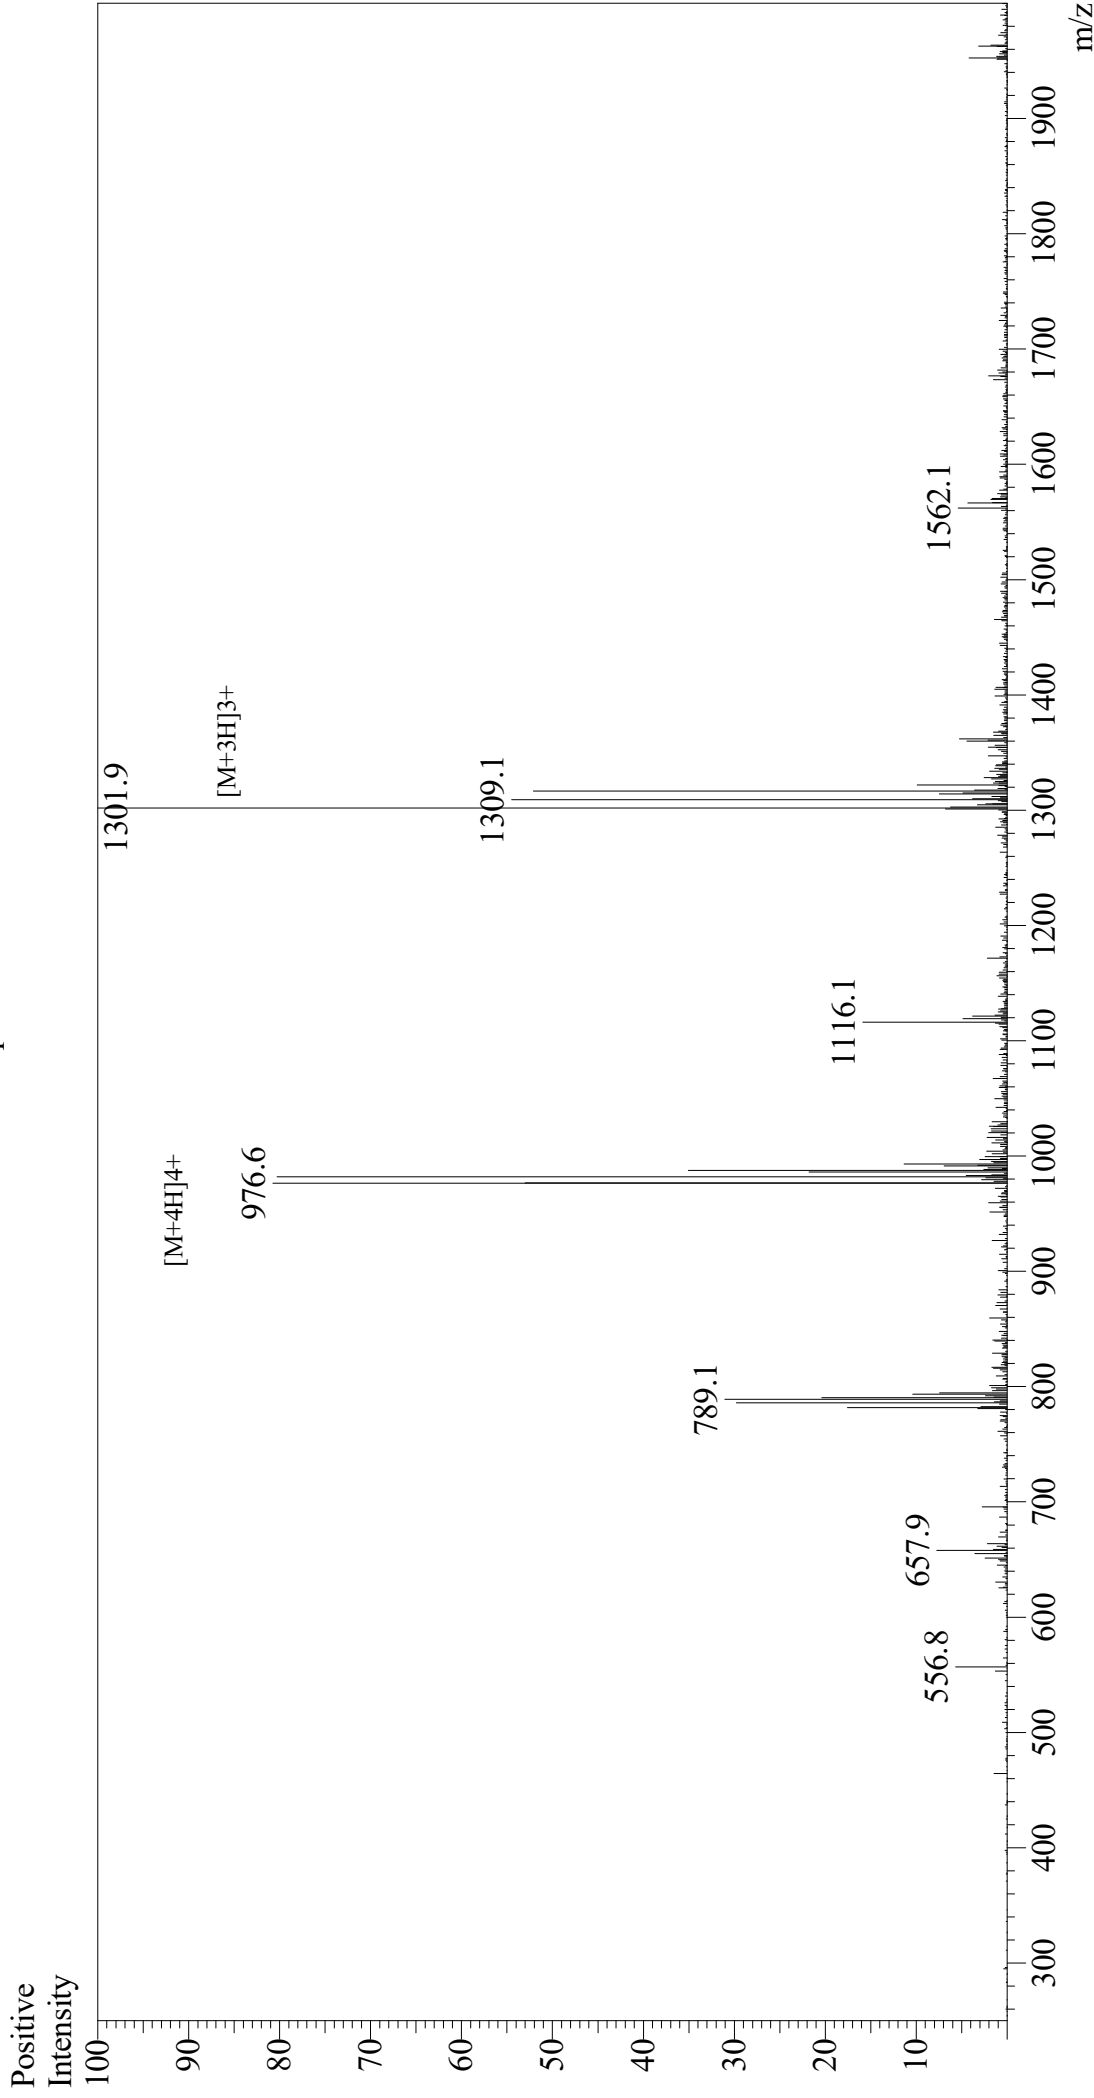

Sample Information
 Month-Day Processed : 12/24/20
 Time Processed : 10:23:38 AM
 Injection Volume : 0.4
 Sample Name : Amylin, human, amide
 Cat No. : RP11278
 Lot No. : E8002020L
 Theoretical MW : 3903.28
 Observed MW : 3902.7

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : GK11010007
 Interface Bias : +3.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H2O/50%MeOH