

Sample Name:C-Peptide (3-33), human
 Cat No:RP11116
 Lot No :E9806820J
 Time Processed :9:11:09 PM
 Month-Day-Year Processed :11/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

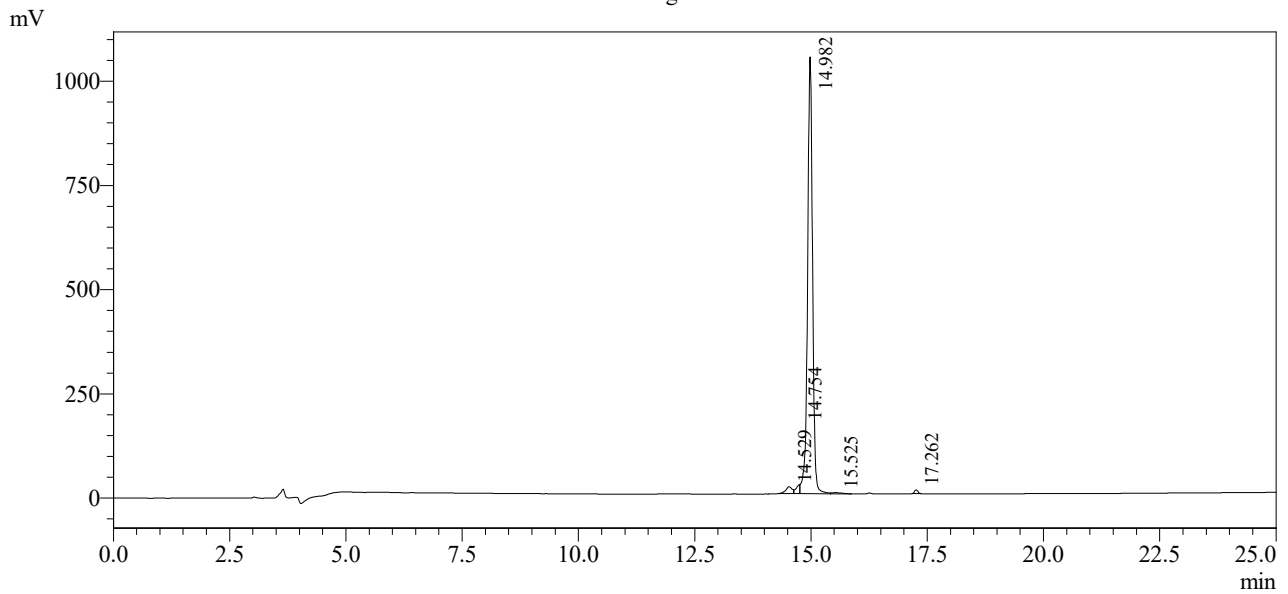

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.529	163057	16510	2.002
2	14.754	116608	21457	1.432
3	14.982	7779819	1047662	95.521
4	15.525	39674	3178	0.487
5	17.262	45475	8908	0.558
Total		8144633	1097715	100.000