

Sample Name :c-Myc Peptide  
 Cat No.: RP11731  
 Lot No.: E4568419K  
 Time Processed :17:13:23  
 Month-Day-Year Processed :11/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
41.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

<Chromatogram>

mV

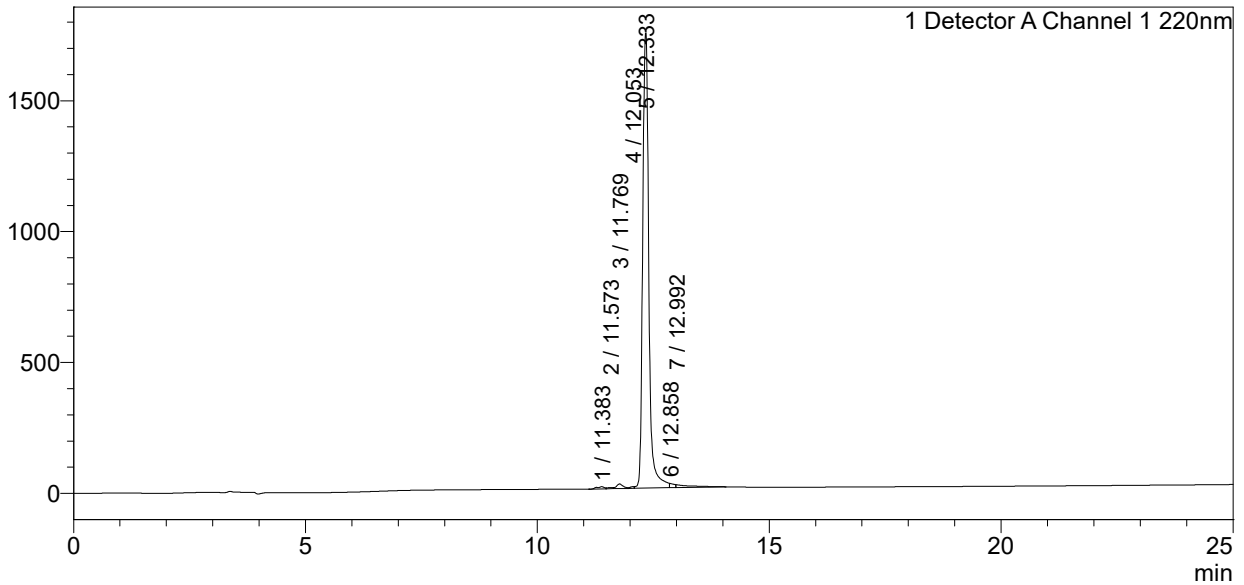

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.383	94959	8430	0.571
2	11.573	38100	4602	0.229
3	11.769	176664	17904	1.061
4	12.053	39803	6311	0.239
5	12.333	15931963	1739274	95.723
6	12.858	110454	16537	0.664
7	12.992	251794	11256	1.513
Total		16643738	1804316	100.000