

Sample Name :DYKDDDDK Peptide  
 Cat. No. : RP10586  
 Lot. No. :E3493019K  
 Time Processed :7:48:15  
 Month-Day-Year Processed :11/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

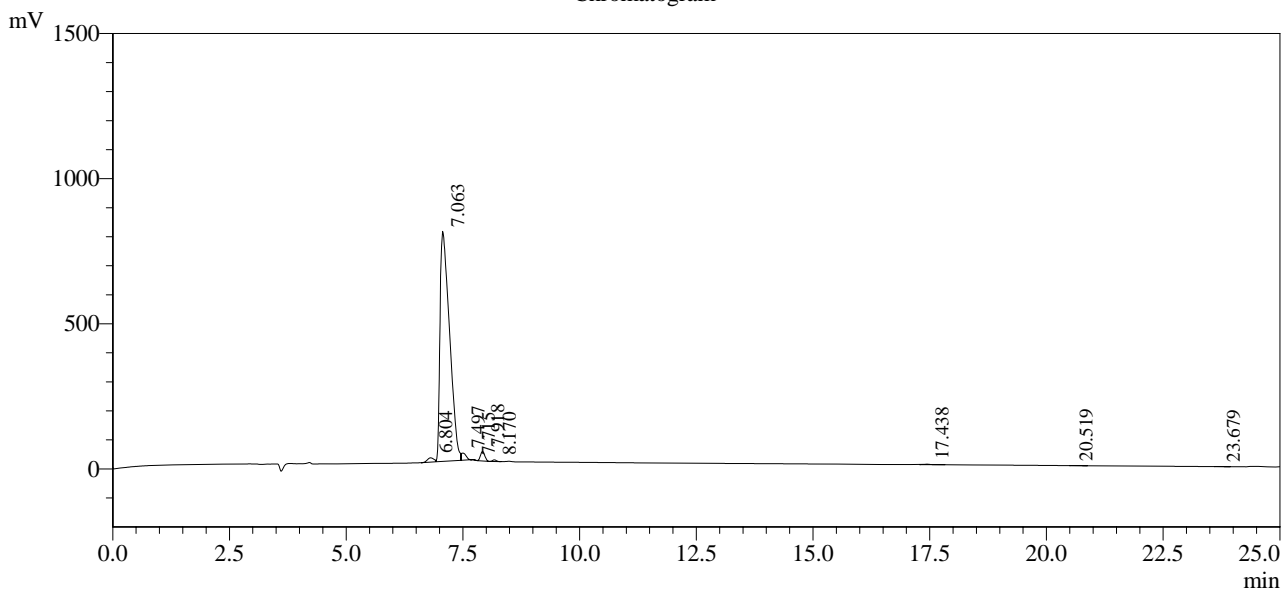

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.804	146919	14945	1.241
2	7.063	11255547	792673	95.091
3	7.497	168764	24493	1.426
4	7.715	8496	1829	0.072
5	7.918	209482	32698	1.770
6	8.170	31303	5627	0.264
7	17.438	13786	1608	0.116
8	20.519	1103	59	0.009
9	23.679	1173	148	0.010
Total		11836573	874079	100.000