


Mass Spectrum

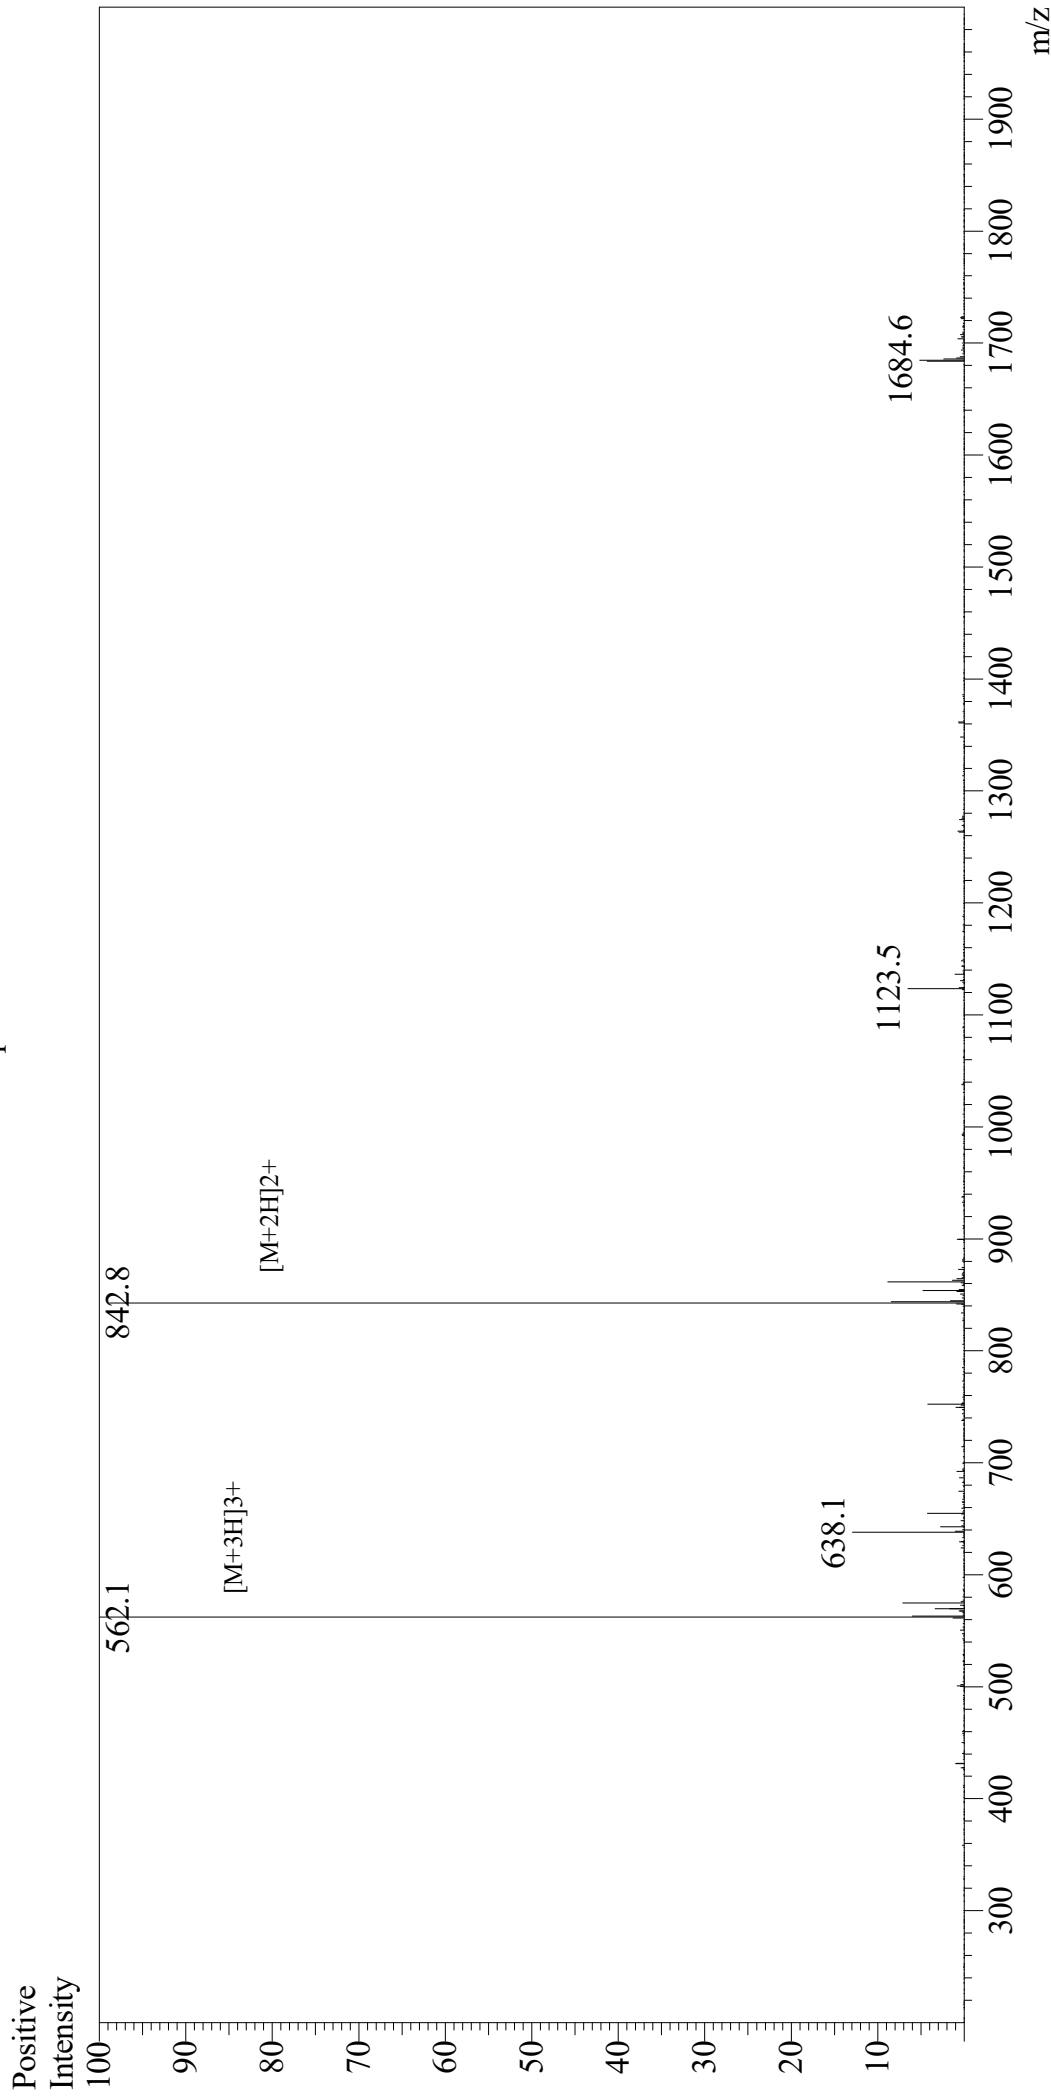

Sample Information

User : Gary
Month-Day Processed : 08/06/20
Time Processed : 10:19:48 AM
Injection Volume : 0.3
Sample Name : α -Factor Mating Pheromone, yeast
Cat No. : RP01002
Lot No. : E6772020H
Theoretical MW : 1683.98
Observed MW : 1683.3

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200