

Sample Name :SV40 T-Ag-derived NLS peptide
 Cat. No. : RP20513
 Lot. No. : PE9021902
 Time Processed :8:52:34
 Month-Day-Year Processed : 03/07/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

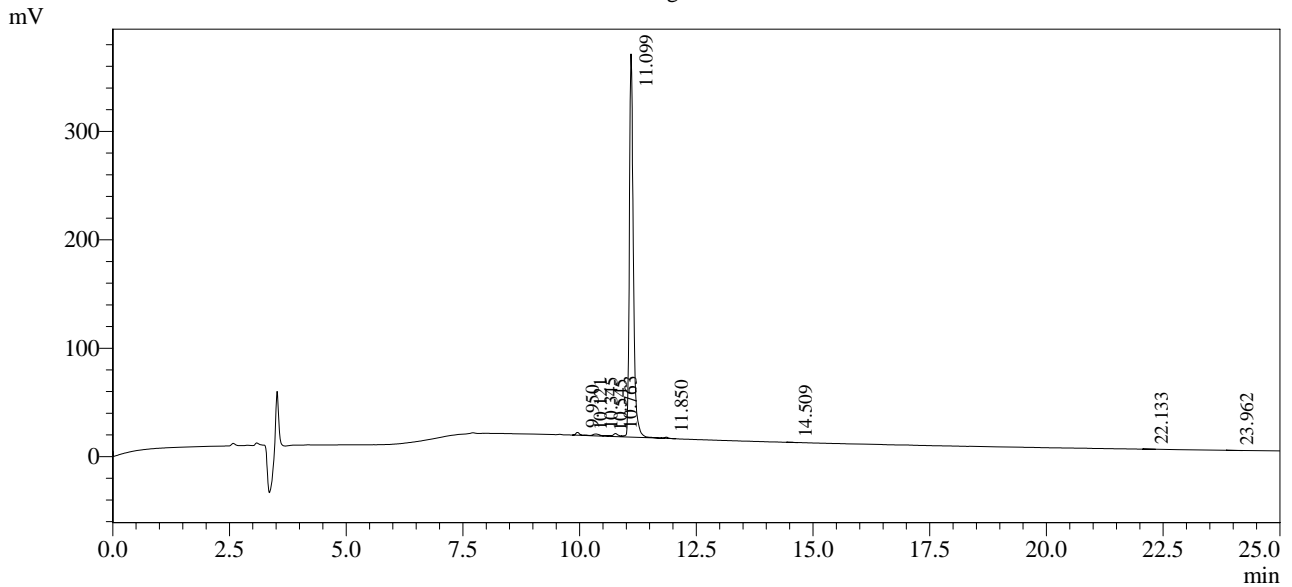

1 Det. A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.950	14409	2597	0.666
2	10.121	2793	455	0.129
3	10.345	17104	1644	0.790
4	10.545	3435	596	0.159
5	10.763	24334	2847	1.124
6	11.099	2092126	353437	96.666
7	11.850	6027	1097	0.278
8	14.509	1154	190	0.053
9	22.133	1266	181	0.058
10	23.962	1639	154	0.076
Total		2164288	363198	100.000