

Sample Name :Palmitoyl Tetrapeptide-3
 Cat No. :RP20100
 Lot No. :E3771921B
 Time Processed : 17:01:36
 Month-Day-Year Processed : 02/14/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

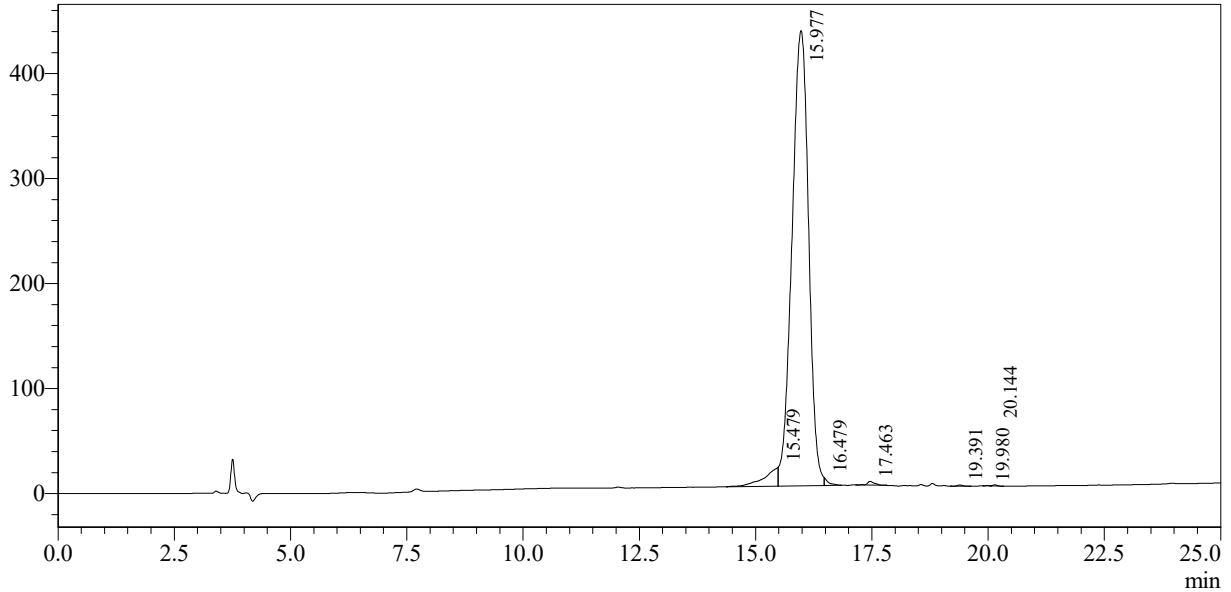

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.479	356046	17440	3.166
2	15.977	10794289	433348	95.994
3	16.479	41451	7367	0.369
4	17.463	36841	3593	0.328
5	19.391	7512	1069	0.067
6	19.980	1498	284	0.013
7	20.144	7134	1146	0.063
Total		11244771	464247	100.000