

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide  
 Cat No.:RP21087  
 Lot No.: E2235020I  
 Time Processed :4:07:08 PM  
 Month-Day-Year Processed :09/21/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: SS-CM-0286

<Chromatogram>  
 Cat No.:

mV

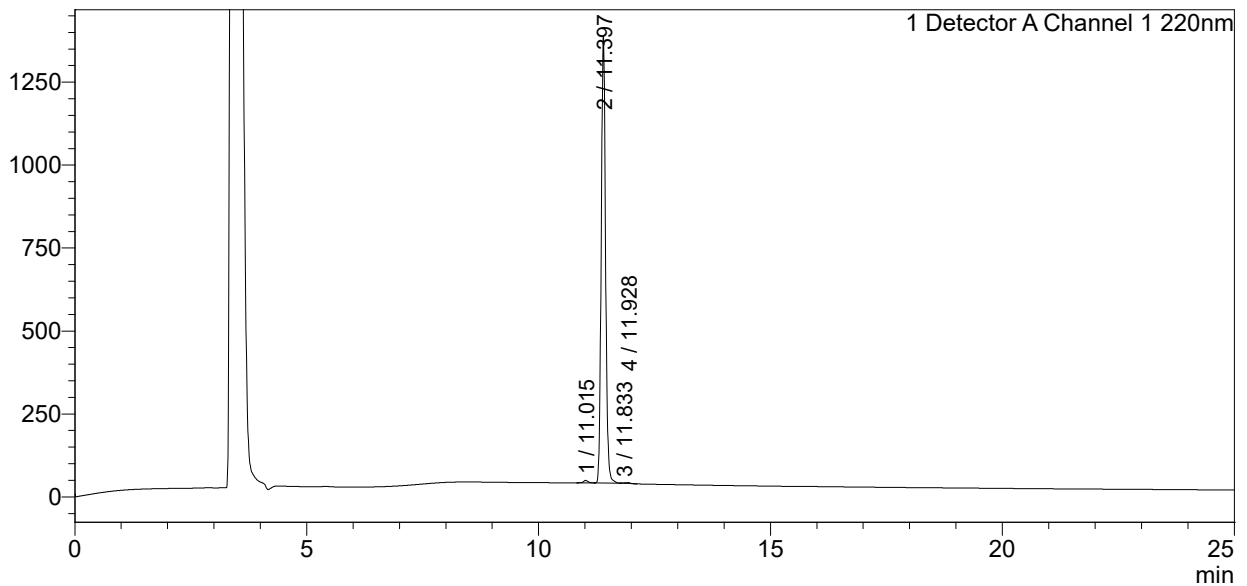

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.015	61686	7845	0.700
2	11.397	8728209	1348840	99.090
3	11.833	3775	849	0.043
4	11.928	14713	2621	0.167
Total		8808382	1360154	100.000