

Sample Name : Glucagon (1-29), Human
 Cat. No.: RP10772
 Lot. No. :E4756619I
 Time Processed :12:13:15
 Month-Day-Year Processed :09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

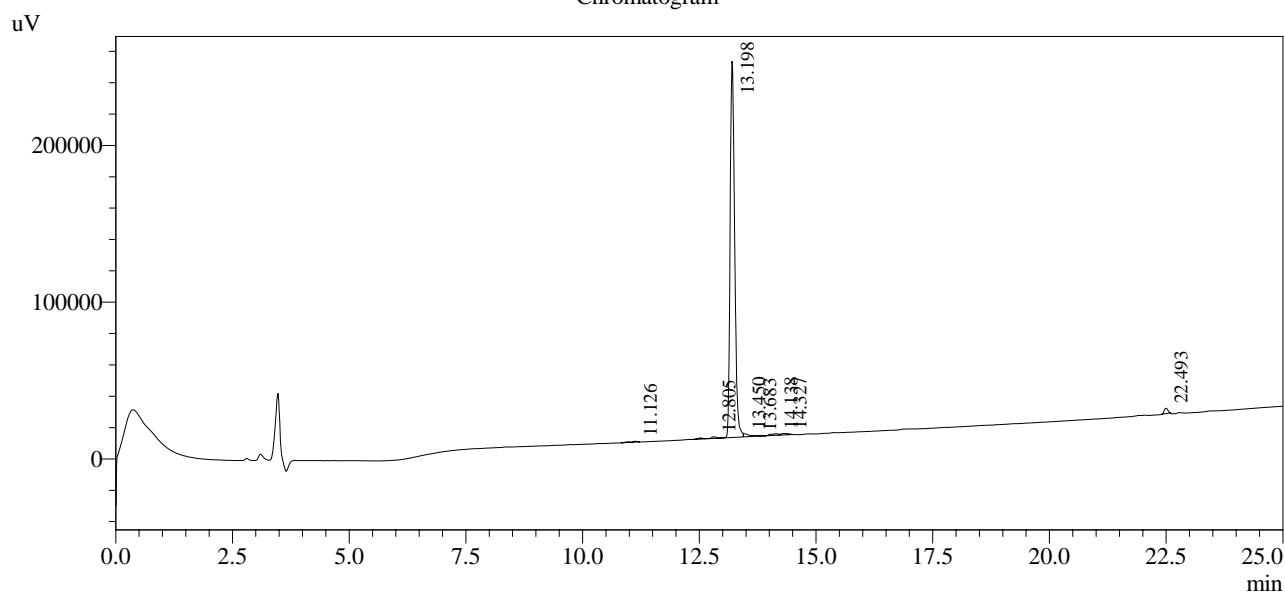

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.126	5760	565	0.338
2	12.805	14267	1098	0.838
3	13.198	1622950	240018	95.320
4	13.450	13689	2097	0.804
5	13.683	4873	557	0.286
6	14.138	12568	1016	0.738
7	14.327	9945	869	0.584
8	22.493	18573	3383	1.091
Total		1702625	249603	100.000