


Sample Name : Hexa-His
 Cat. No. : RP11737
 Lot. No. : E0401920D
 Time Processed : 13:46:37
 Month-Day-Year Processed : 04/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	0	
5.00	Pumps	Pump B Conc.	0	
20.00	Pumps	Pump B Conc.	30	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	0	
40.00	Pumps	Pump B Conc.	0	
40.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

Chromatogram

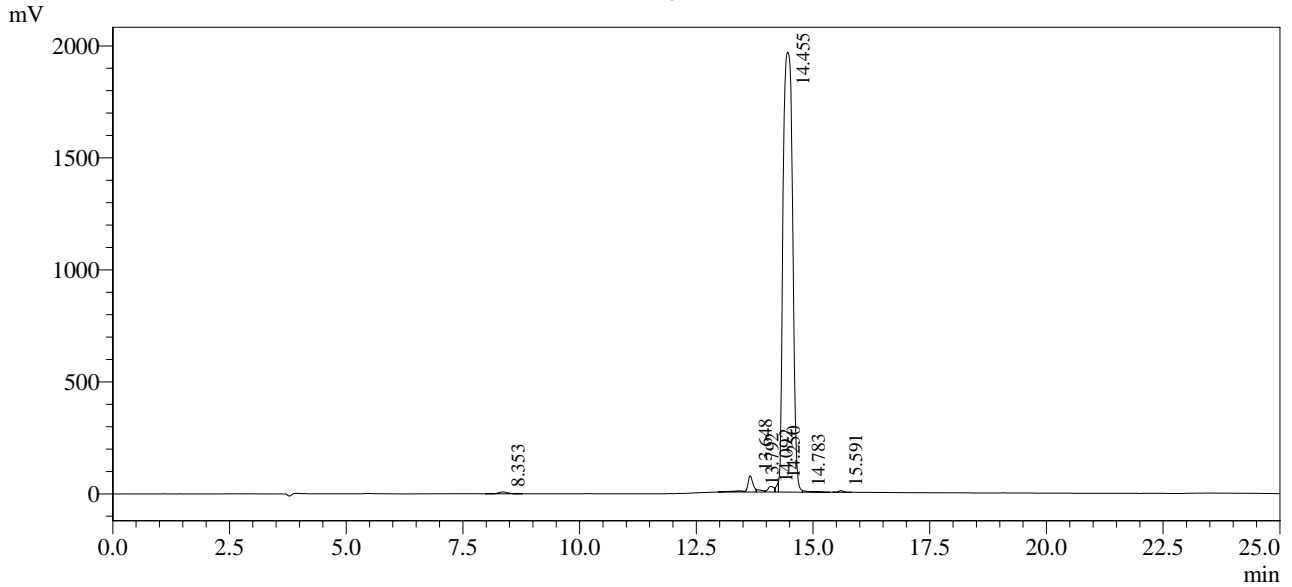

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.353	116467	8637	0.399
2	13.648	622001	72970	2.129
3	13.792	90579	10669	0.310
4	14.092	222198	25253	0.760
5	14.250	138384	39708	0.474
6	14.455	27910615	1964856	95.513
7	14.783	70697	6859	0.242
8	15.591	50727	7365	0.174
Total		29221669	2136317	100.000