

Sample Name :PAR-4 Agonist Peptide, amide
 Cat No. :RP11529
 Lot No. :E7716820H
 Time Processed: 9:14:48
 Month-Day-Year Processed :08/13/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

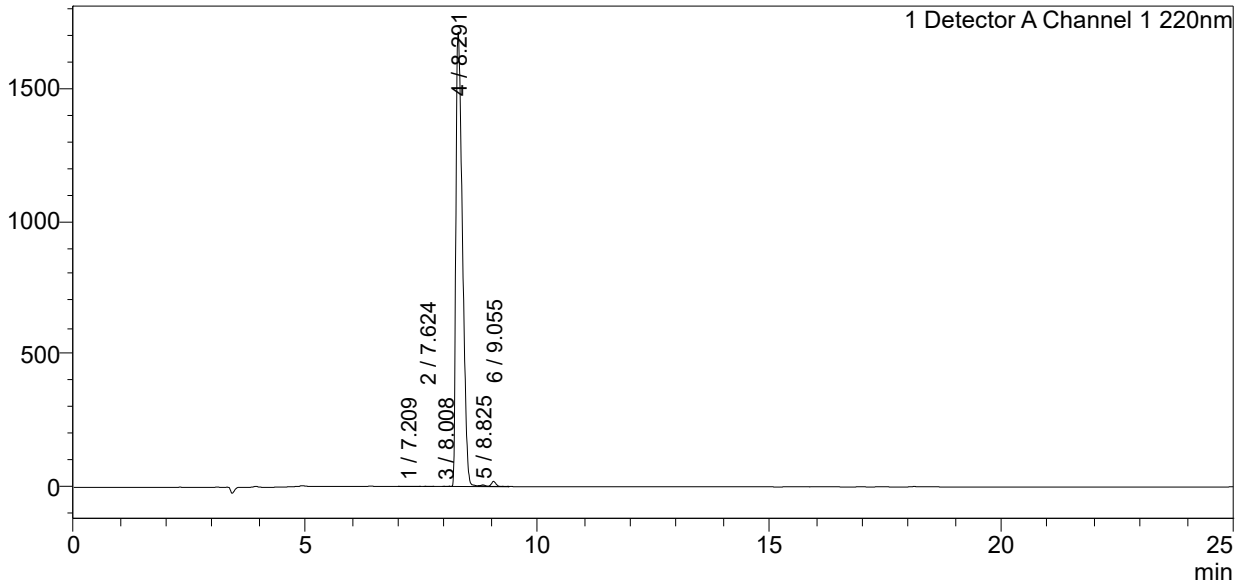

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.209	6346	501	0.037
2	7.624	2495	518	0.015
3	8.008	1056	184	0.006
4	8.291	16829147	1706470	99.072
5	8.825	26139	4450	0.154
6	9.055	121676	18662	0.716
Total		16986859	1730784	100.000