

Sample Name :β-Amyloid (25-35)
 Cat. No. : RP10008
 Lot. No. : E0751519G
 Time Processed :8:21:43
 Month-Day-Year Processed :08/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment :SS-CM-0310

Chromatogram

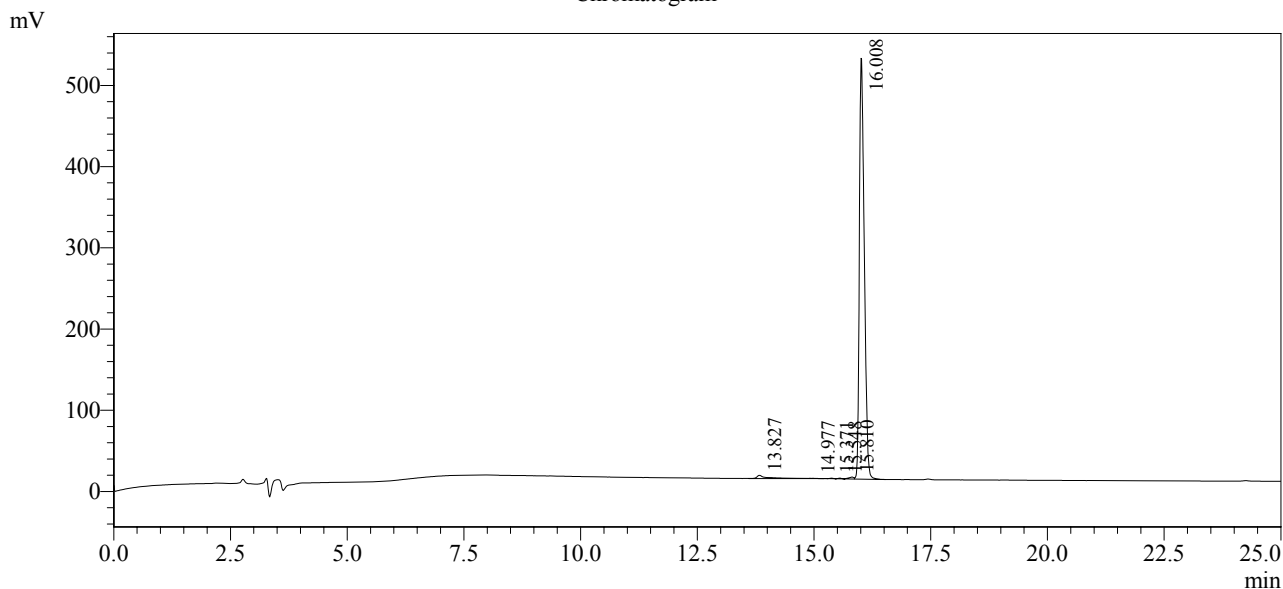

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.827	68753	3922	1.763
2	14.977	1589	231	0.041
3	15.371	2869	603	0.074
4	15.548	3752	751	0.096
5	15.810	17385	2360	0.446
6	16.008	3806267	518189	97.581
Total		3900615	526056	100.000