

Sample Name :Hexa-His
 Cat No.: RP11737
 Lot No.: E7553320B
 Time Processed :16:58:12
 Month-Day-Year Processed :02/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
25.00	Pumps	Pump A B.Conc	50
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	0
40.00	Pumps	Pump A B.Conc	0
40.00	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

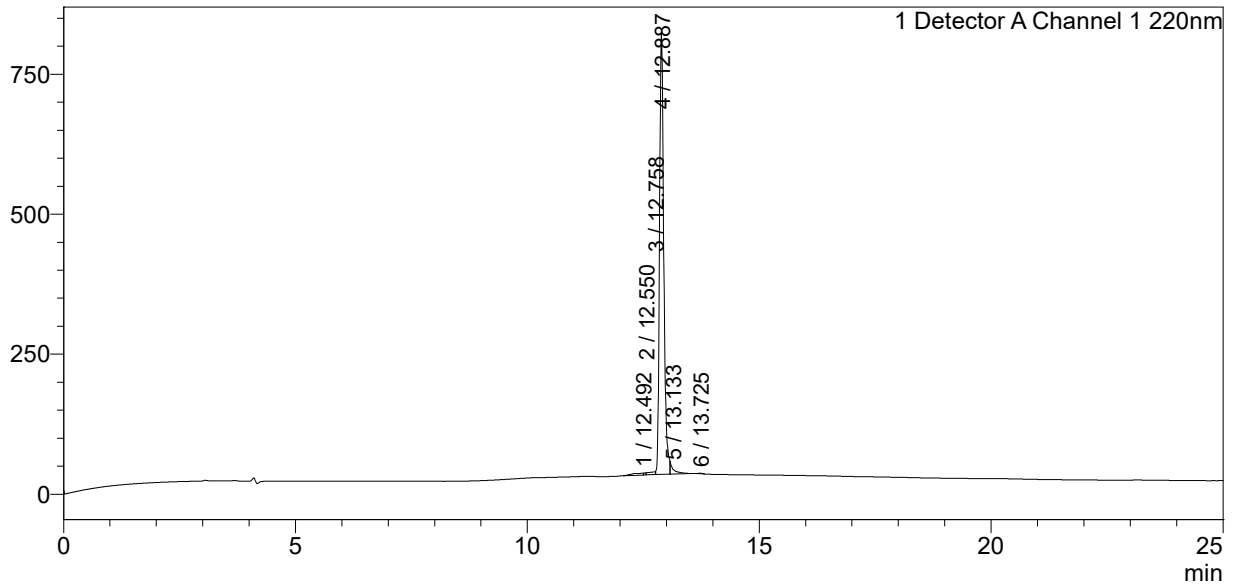

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.492	56524	3283	1.072
2	12.550	12692	3765	0.241
3	12.758	55590	5078	1.055
4	12.887	5031603	788630	95.465
5	13.133	109007	9537	2.068
6	13.725	5235	935	0.099
Total		5270649	811228	100.000