

Sample Name :OVA Peptide (323-339)
 Cat. No. : RP10610
 Lot. No. : PE2301905
 Time Processed : 8:51:46
 Month-Day-Year Processed : 05/25/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

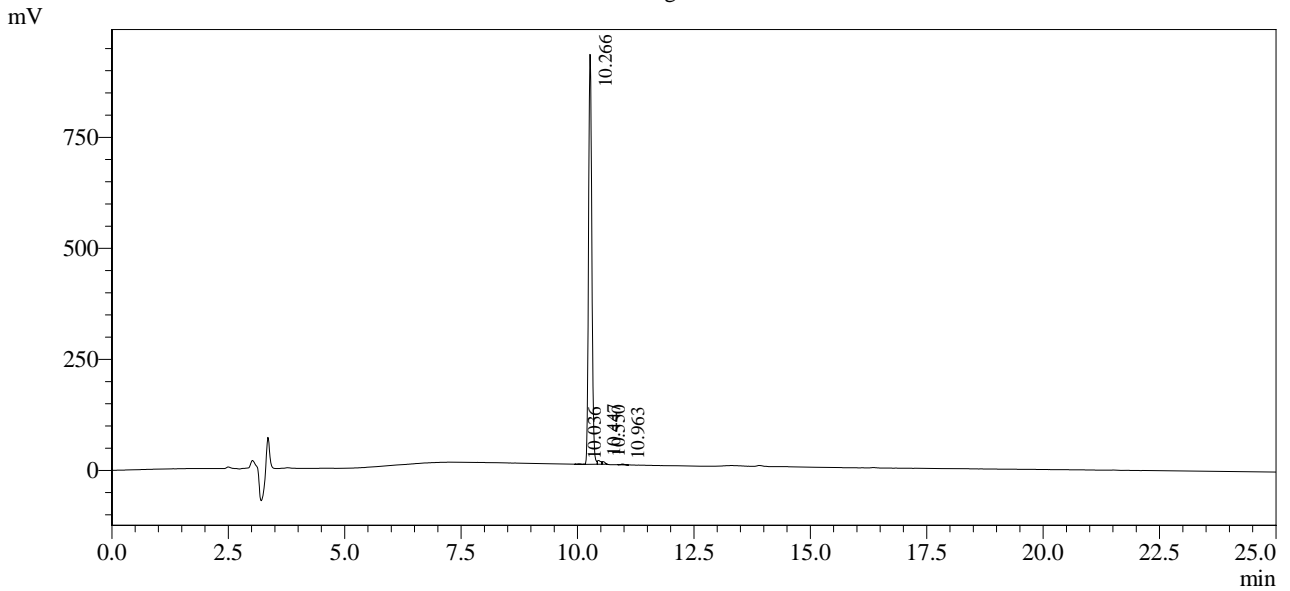

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.036	4027	899	0.087
2	10.266	4561365	923022	98.329
3	10.447	41038	8314	0.885
4	10.550	23362	5743	0.504
5	10.963	9111	1874	0.196
Total		4638902	939852	100.000