

Sample Name : Hexa-His
 Cat. No. : RP11737
 Lot. No. : E7080019K
 Time Processed :7:52:32
 Month-Day-Year Processed :11/29/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

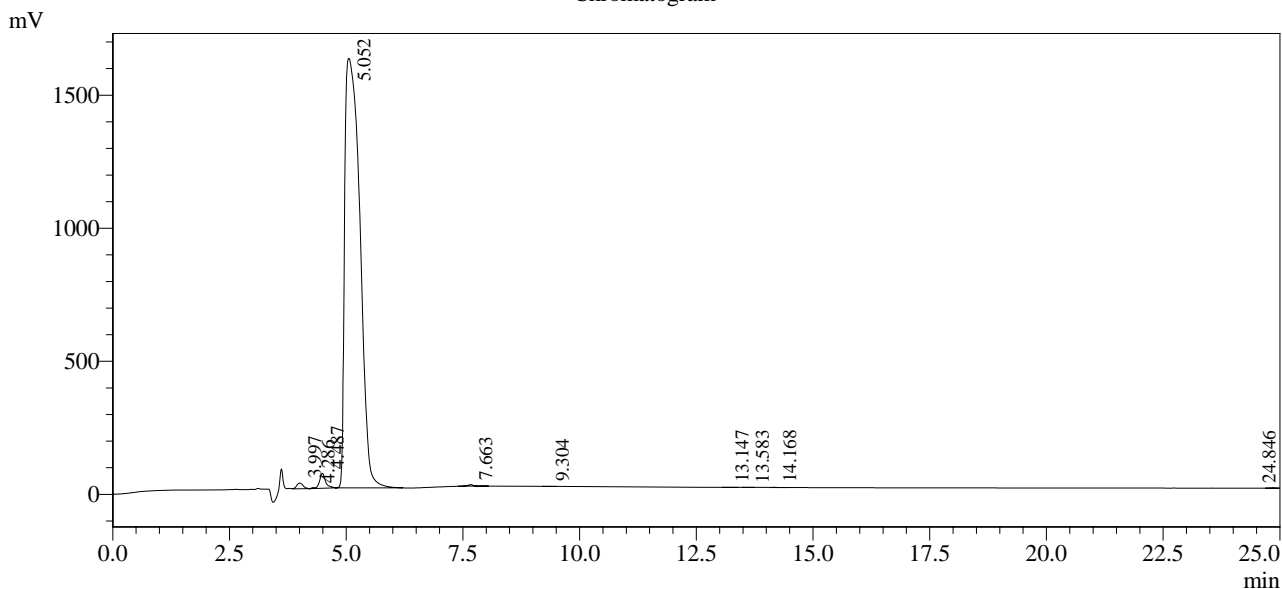

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	3.997	199816	21180	0.538
2	4.286	15710	3722	0.042
3	4.487	487327	56404	1.311
4	5.052	36389030	1614197	97.922
5	7.663	51640	5884	0.139
6	9.304	3376	549	0.009
7	13.147	1793	290	0.005
8	13.583	1791	336	0.005
9	14.168	4859	871	0.013
10	24.846	6061	791	0.016
Total		37161402	1704224	100.000