

Sample Name :Glucagon (1-29), Human  
 Cat No.: RP10772  
 Lot No.: PE6861811  
 Time Processed:16:05:19  
 Month-Day-Year Processed:11/28/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

<Chromatogram>

mV

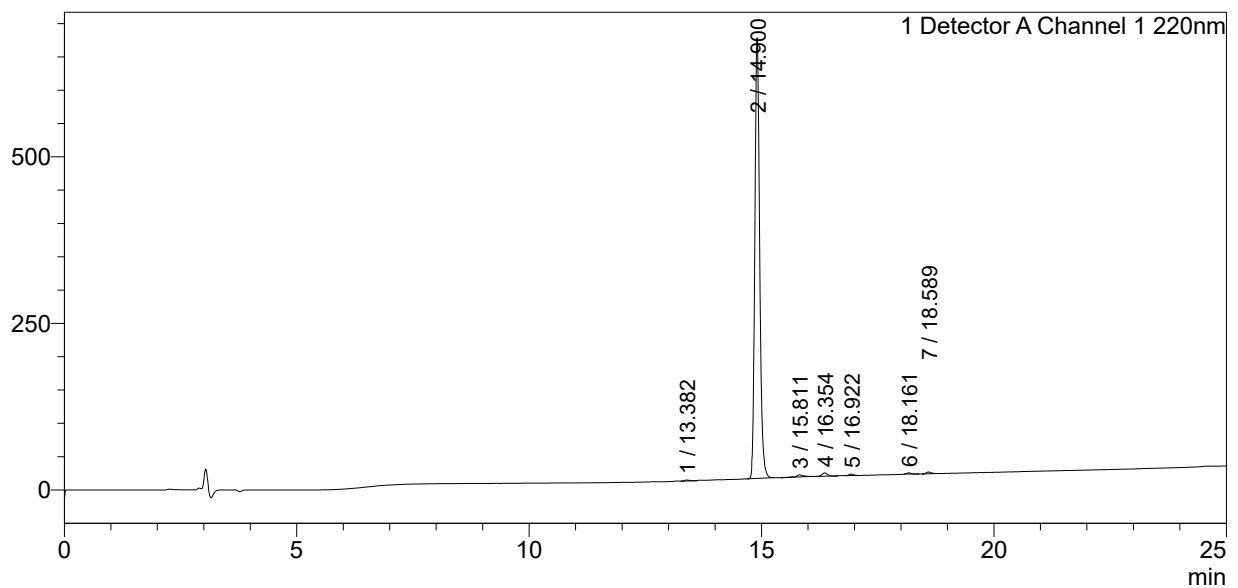

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.382	10961	1361	0.223
2	14.900	4793115	660967	97.408
3	15.811	34836	3259	0.708
4	16.354	37741	4930	0.767
5	16.922	13955	2120	0.284
6	18.161	11079	1759	0.225
7	18.589	18946	2586	0.385
Total		4920633	676982	100.000