

Sample Name :hgp100(25-33)  
 Cat. No. :RP20344  
 Lot. No. :PE2541803

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

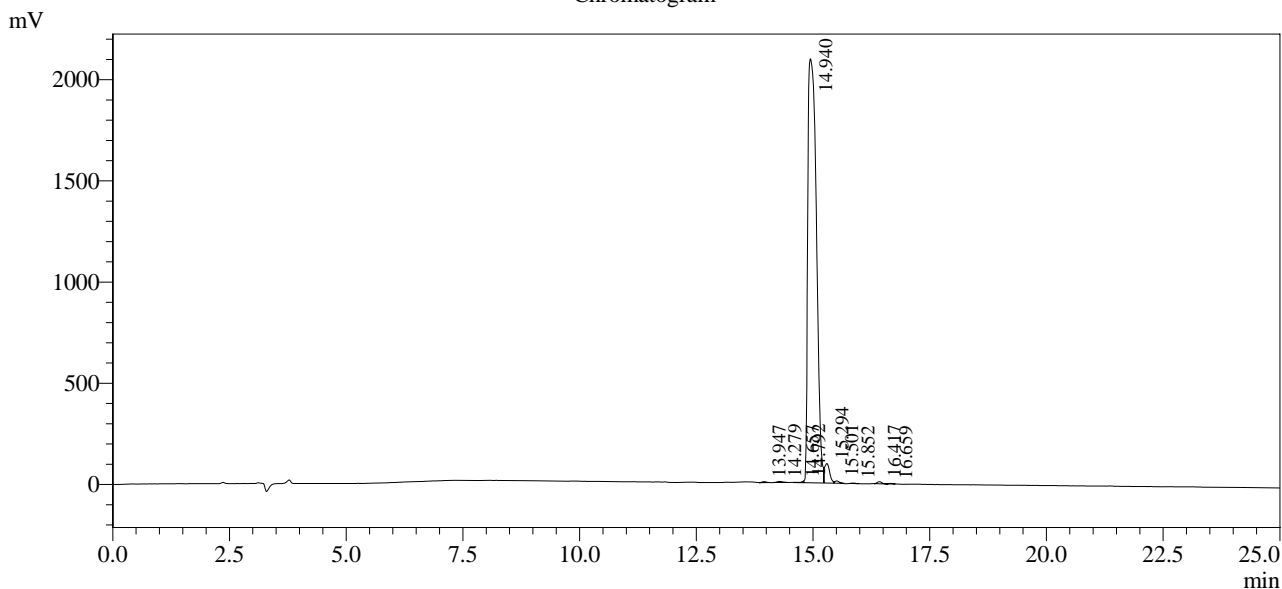

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.947	28005	4652	0.101
2	14.279	34794	4806	0.125
3	14.657	13087	2171	0.047
4	14.792	20556	7021	0.074
5	14.940	26825277	2095019	96.421
6	15.294	723463	96877	2.600
7	15.501	74204	11341	0.267
8	15.852	13986	2842	0.050
9	16.417	72057	10432	0.259
10	16.659	15573	3097	0.056
Total		27821000	2238257	100.000