

Sample Name: Calcitonin Gene Related Peptide (CGRP) (8-37), rat  
 Cat No : RP11090  
 Lot No : E6948821E  
 Time Processed : 20:04:59  
 Month-Day-Year Processed : 05/23/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment : SS-CM-0309

<Chromatogram>

mV

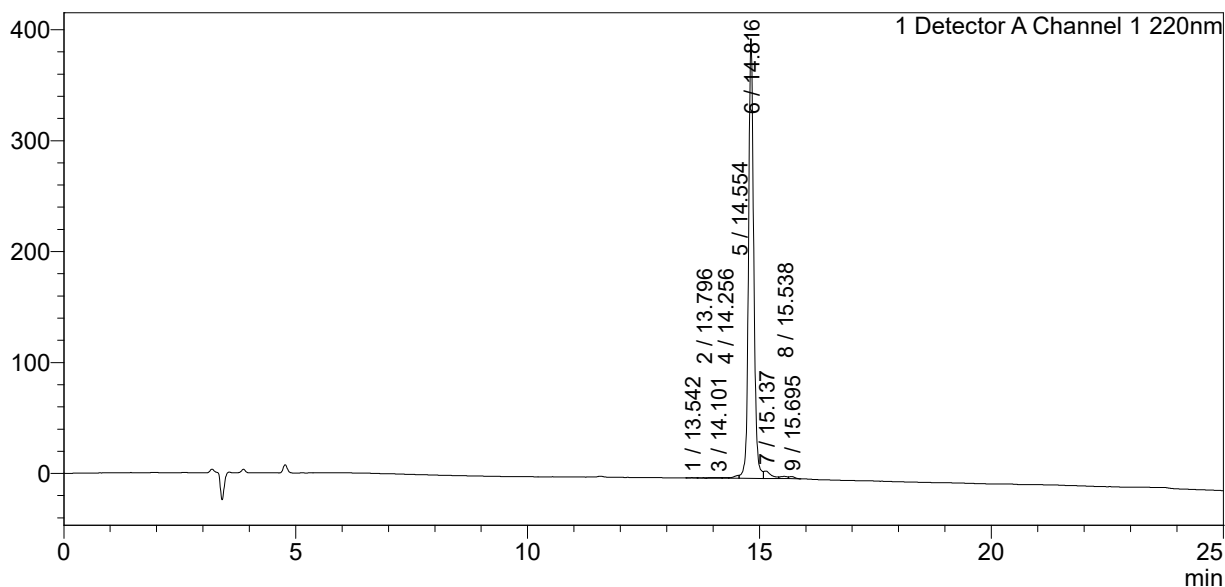

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.542	2004	218	0.061
2	13.796	2676	289	0.082
3	14.101	9820	614	0.301
4	14.256	5211	647	0.160
5	14.554	19968	2665	0.613
6	14.816	3106393	396492	95.329
7	15.137	74394	6696	2.283
8	15.538	22293	2017	0.684
9	15.695	15844	1968	0.486
Total		3258603	411605	100.000