

Sample Name :C-Type Natriuretic Peptide (CNP) (1-22), human
 Cat. No. : RP11110
 Lot. No. : PE3321904
 Time Processed : 11:04:50
 Month-Day-Year Processed : 04/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

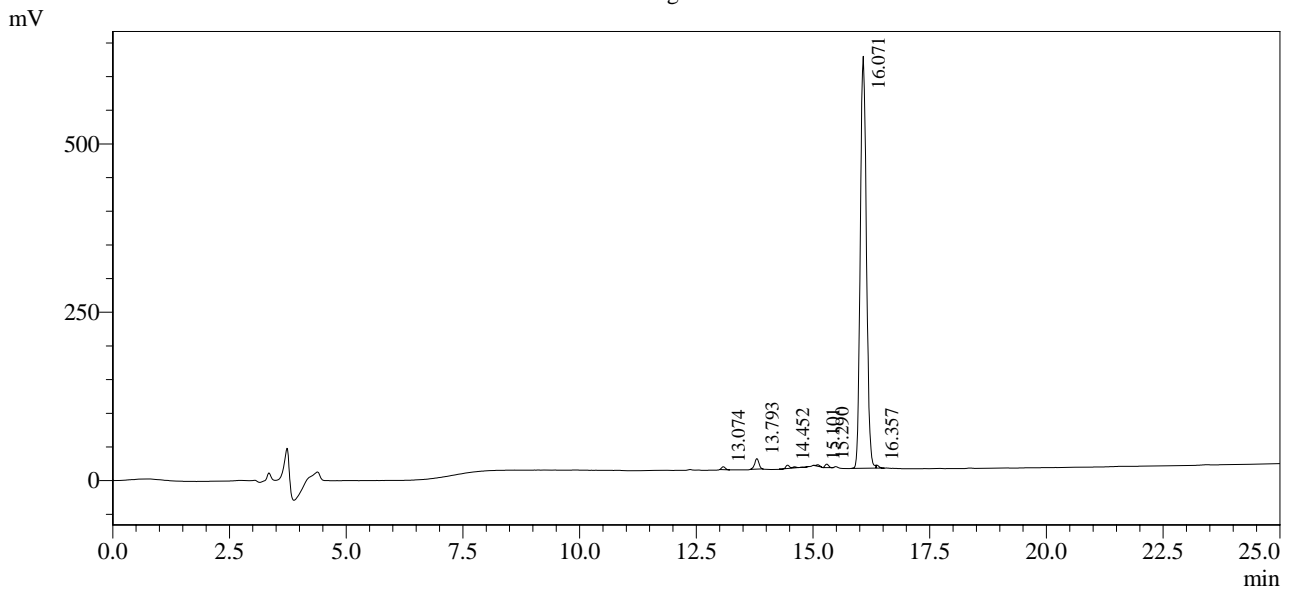

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.074	24204	4295	0.416
2	13.793	98323	15583	1.691
3	14.452	32900	5045	0.566
4	15.101	11151	2246	0.192
5	15.290	25821	5133	0.444
6	16.071	5602602	611930	96.382
7	16.357	17931	4601	0.308
Total		5812931	648833	100.000