

Sample Name :C-Type Natriuretic Peptide (CNP) (1-22), human  
 Cat No.: RP11110  
 Lot No.: E4792919I  
 Time Processed :20:12:51  
 Month-Day-Year Processed :09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
31.00	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

<Chromatogram>

mV

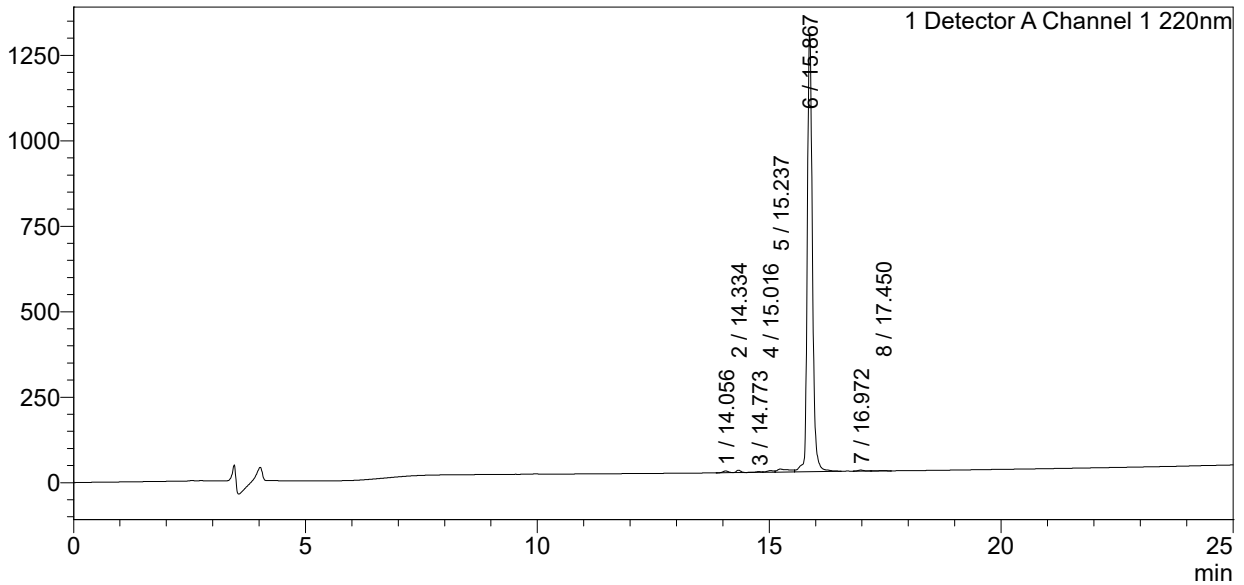

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.056	41586	5186	0.411
2	14.334	46469	7124	0.459
3	14.773	18947	1907	0.187
4	15.016	46336	4276	0.458
5	15.237	159803	8553	1.580
6	15.867	9768913	1283356	96.563
7	16.972	24243	2981	0.240
8	17.450	10367	806	0.102
Total		10116663	1314188	100.000