

Sample Name : Flagelin22
 Cat. No. : RP19986
 Lot. No. : PE7331612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
10.00	Pumps	Pump B Conc.	35	
35.00	Pumps	Pump B Conc.	95	
41.00	Pumps	Pump B Conc.	95	
41.01	Pumps	Pump B Conc.	5	
50.00	Pumps	Pump B Conc.	5	
50.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

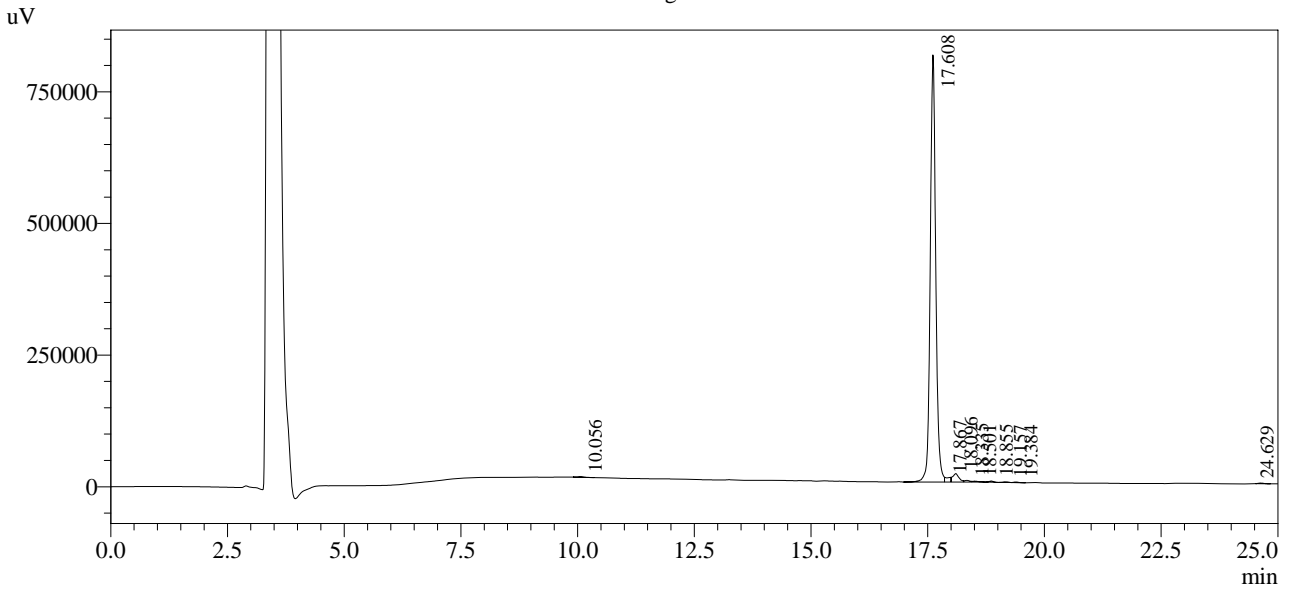

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.056	8965	1130	0.129
2	17.608	6627649	811206	95.483
3	17.867	71783	8897	1.034
4	18.096	148830	16014	2.144
5	18.335	26209	3278	0.378
6	18.501	17833	1789	0.257
7	18.855	13919	2334	0.201
8	19.157	8673	1359	0.125
9	19.384	7440	1143	0.107
10	24.629	9857	1177	0.142
Total		6941159	848327	100.000