

Sample Name : β -Amyloid (25-35)
 Cat No. :RP10008
 Lot No. :E9582619L
 Time Processed :7:51:29
 Month-Day-Year Processed :12/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

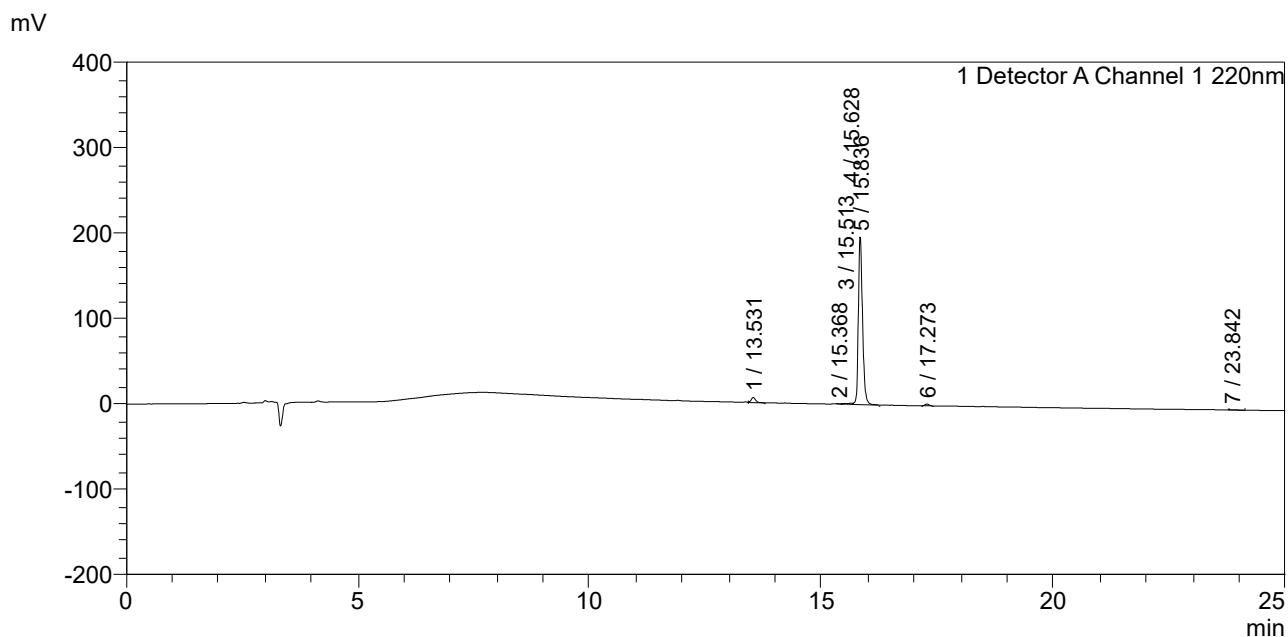

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.531	39701	5958	3.072
2	15.368	312	126	0.024
3	15.513	3676	681	0.284
4	15.628	7318	1244	0.566
5	15.836	1227813	196120	95.003
6	17.273	12163	2093	0.941
7	23.842	1406	134	0.109
Total		1292389	206356	100.000