

Sample Name :Exendin-4
 Cat. No. :RP10874
 Lot. No. :PE5241901
 Time Processed : 17:06:17
 Month-Day-Year Processed : 01/12/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
45.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

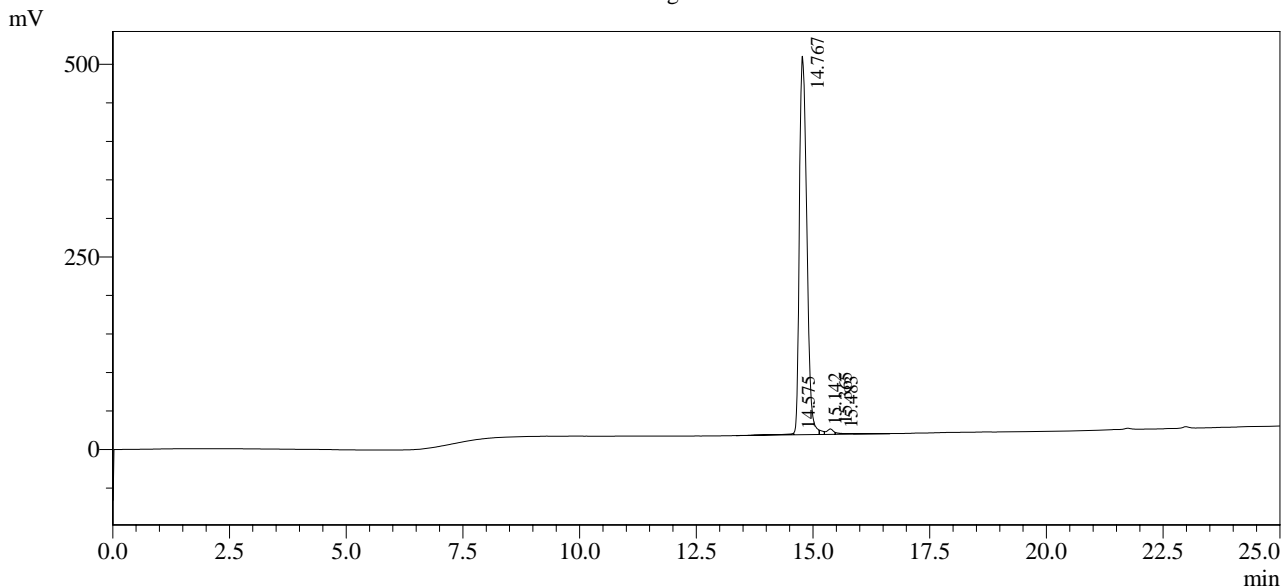

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.575	42237	1946	0.754
2	14.767	5423792	491274	96.826
3	15.142	29641	5681	0.529
4	15.365	69098	7191	1.234
5	15.483	36826	2340	0.657
Total		5601595	508431	100.000