

Sample Name :Hexa-His
 Cat No. :RP11737
 Lot No. :E3862720I
 Time Processed :11:10:51
 Month-Day-Year Processed :06/25/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
25.00	Pumps	Pump A B.Conc	50
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	0
40.00	Pumps	Pump A B.Conc	0
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

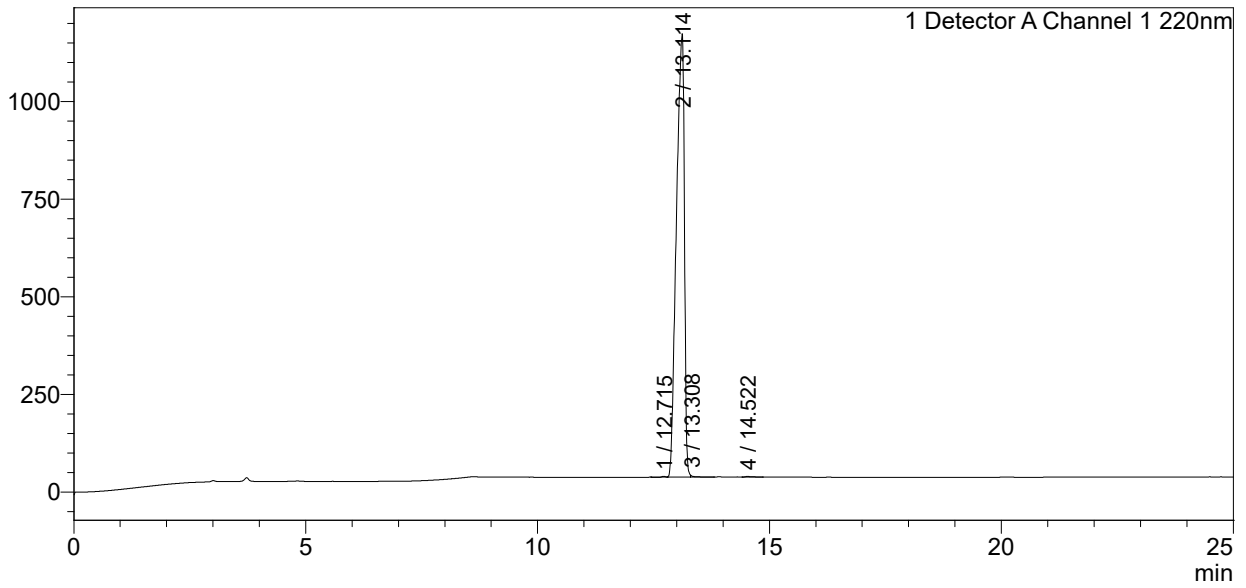

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.715	3313	2256	0.025
2	13.114	13453476	1135509	99.725
3	13.308	16943	3867	0.126
4	14.522	16862	1569	0.125
Total		13490593	1143201	100.000