

Sample Name : β -Amyloid (1-40)
 Cat No :RP10004
 Lot No :E8971520J
 Time Processed :5:15:57 PM
 Month-Day-Year Processed :11/14/2020


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.10	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

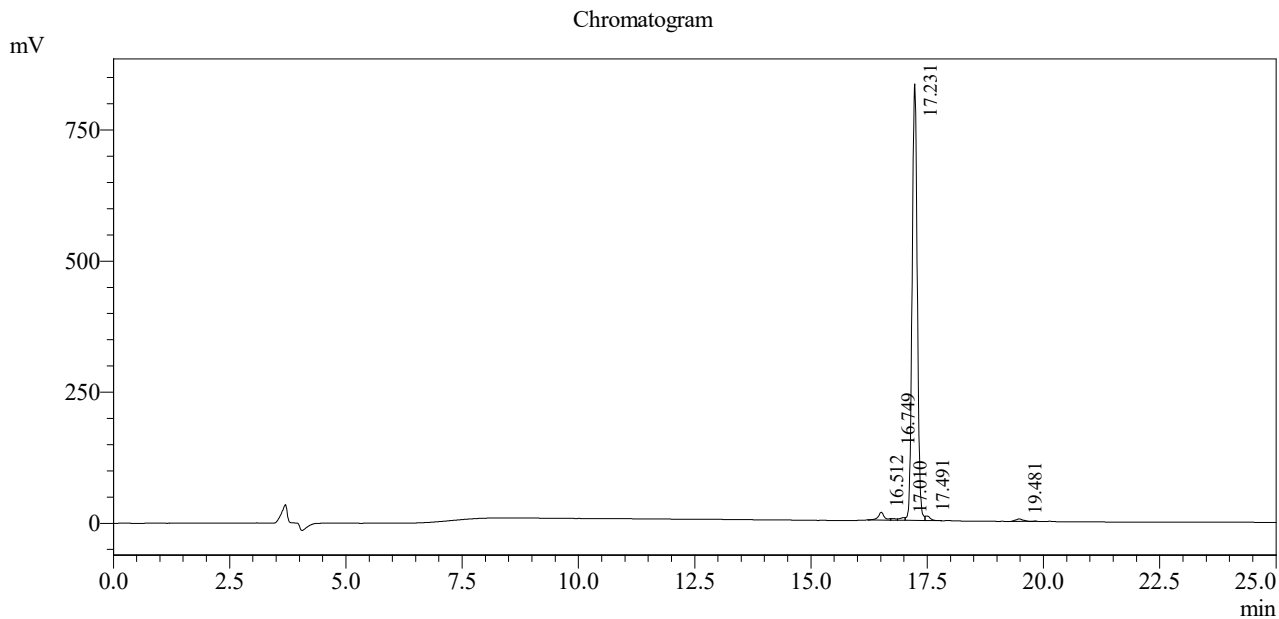

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.512	140000	14959	2.064
2	16.749	24220	2944	0.357
3	17.010	41502	5332	0.612
4	17.231	6465429	832708	95.306
5	17.491	64722	8813	0.954
6	19.481	48024	4665	0.708
Total		6783896	869421	100.000