

Sample Name :GLP-1 (7-36), amide, human
 Cat. No. :RP10773 Lot. No. : PE8021810
 Time Processed : 9:53:16
 Month-Day-Year Processed : 10/31/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

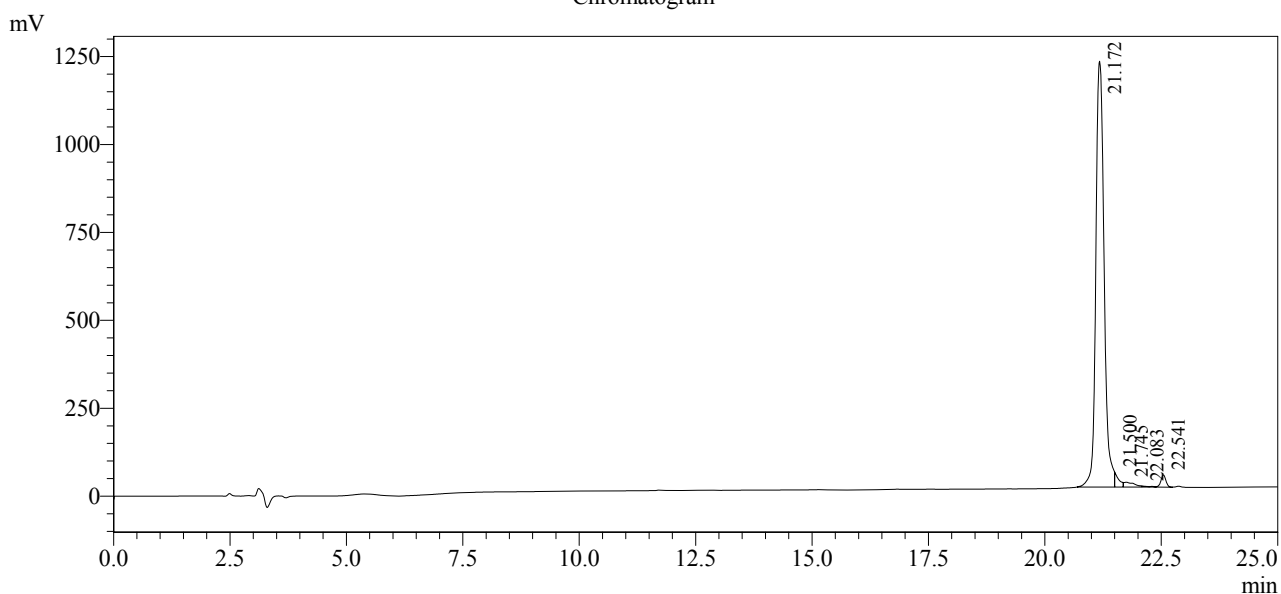

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	21.172	14890232	1210806	95.174
2	21.500	246273	43137	1.574
3	21.745	218537	13674	1.397
4	22.083	30920	3273	0.198
5	22.541	259329	34840	1.658
Total		15645290	1305731	100.000