

Sample Name:C-Type Natriuretic Peptide (CNP) (1-22), human
 Cat No.: RP11110
 Lot No.:E9584119L
 Time Processed :14:35:42
 Month-Day-Year Processed :12/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
30.00	Pumps	Pump A B.Conc	95
30.10	Pumps	Pump A B.Conc	95
35.00	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

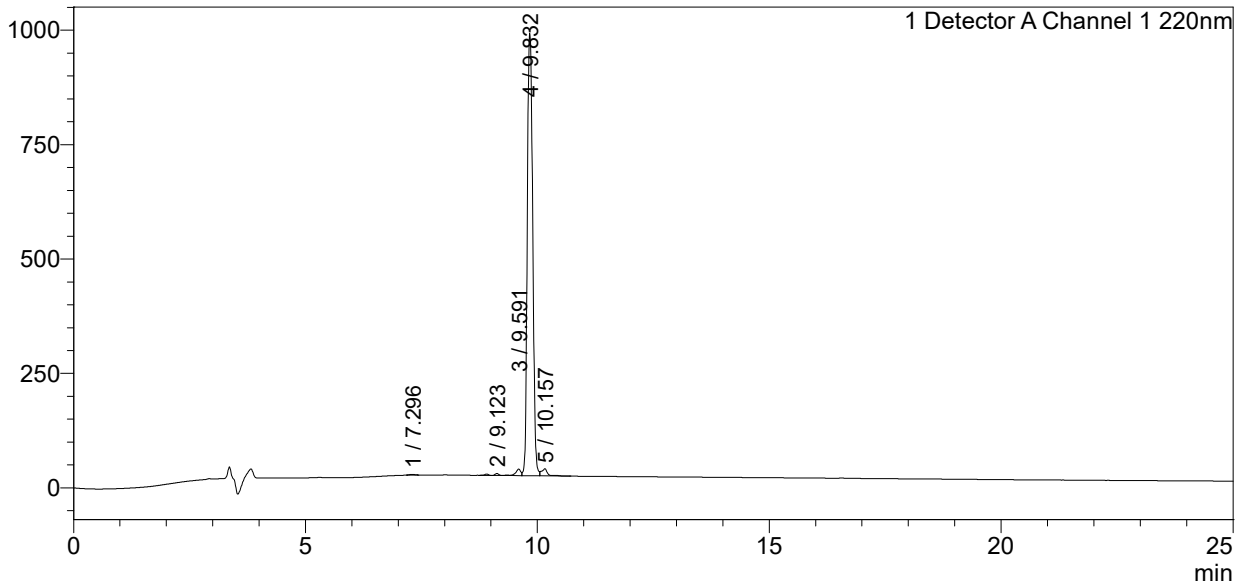

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.296	11423	1519	0.141
2	9.123	43575	4283	0.539
3	9.591	105318	14371	1.302
4	9.832	7788194	967843	96.252
5	10.157	142918	15573	1.766
Total		8091429	1003590	100.000