


Mass Spectrum

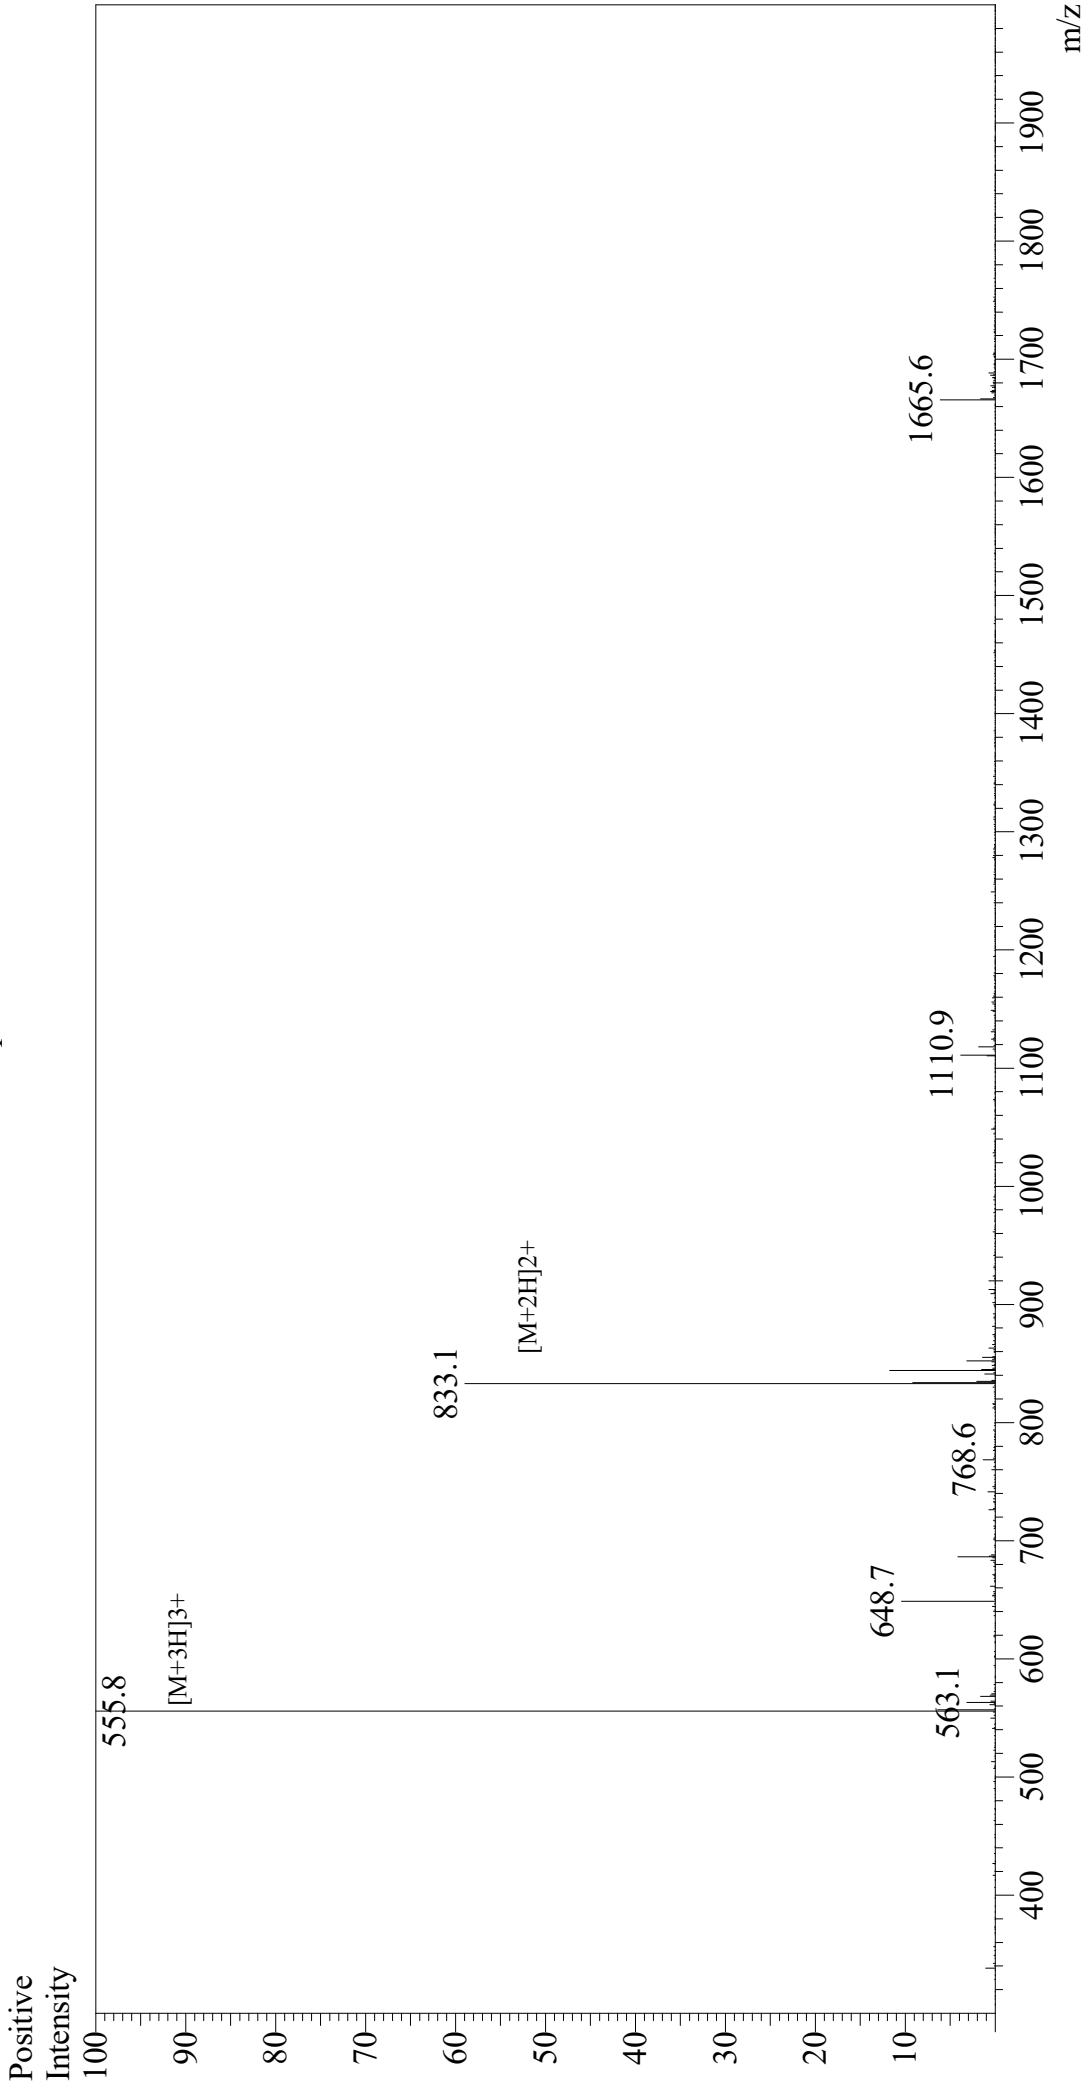

Sample Information
Month-Day Processed : 10/15/20
Time Processed : 10:24:30 PM
Injection Volume : 0.3
Sample Name : α -Melanocyte-Stimulating Hormone (MSH), amide
Cat. No. : RP10644
Lot. No. : E2529220J
Theoretical MW : 1664.90
Observed MW : 1664.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH