

Sample Name :CEF20  
 Cat No. :RP11781  
 Lot No. :E0053719H  
 Time Processed :8:53:38  
 Month-Day-Year Processed :08/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

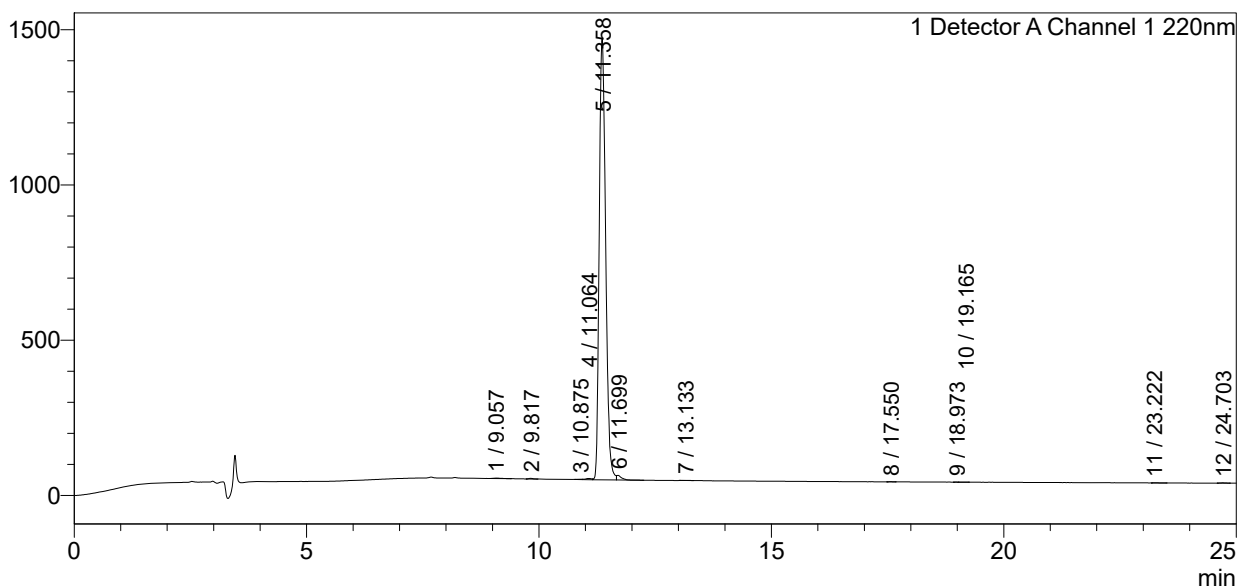

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.057	14910	1030	0.108
2	9.817	13877	2108	0.100
3	10.875	6005	891	0.043
4	11.064	35687	3810	0.258
5	11.358	13643662	1420860	98.597
6	11.699	106536	14876	0.770
7	13.133	3015	393	0.022
8	17.550	2056	333	0.015
9	18.973	1044	286	0.008
10	19.165	1498	235	0.011
11	23.222	2655	217	0.019
12	24.703	6895	868	0.050
Total		13837840	1445906	100.000