

Sample Name:β-Amyloid (1-42), human
 Cat No. :RP10017
 Lot No. :E2021021C
 Time Processed :12:19:53 PM
 Month-Day-Year Processed :04/09/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	10
25.00	Pumps	B.Conc	100
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

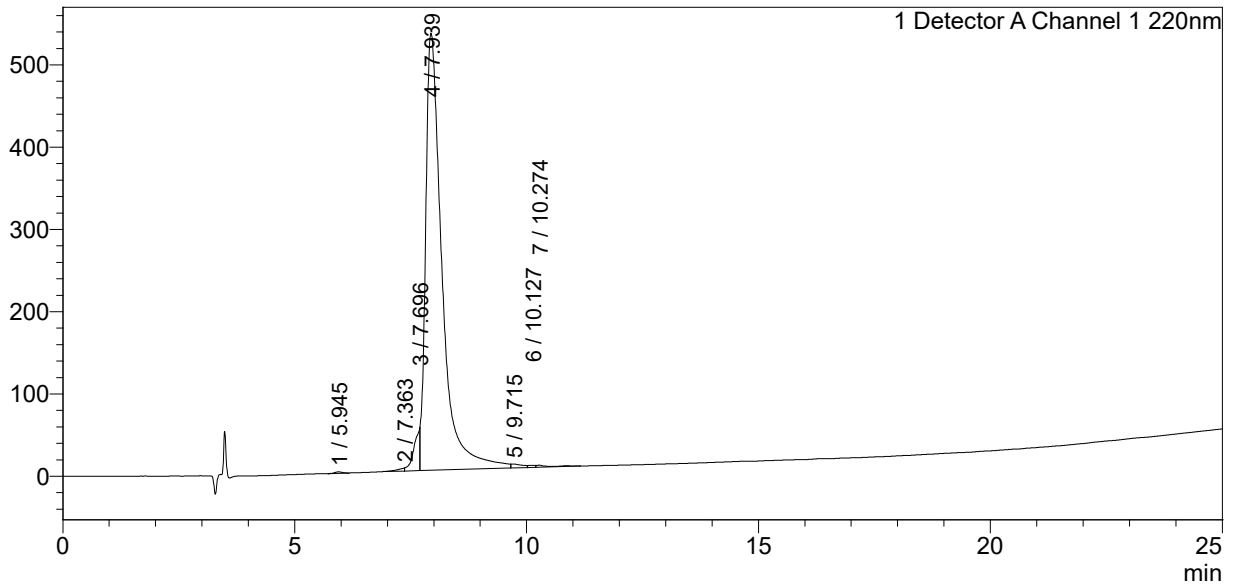

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.945	18445	1715	0.135
2	7.363	38104	3585	0.279
3	7.696	458962	50077	3.364
4	7.939	12983361	531346	95.149
5	9.715	76051	4656	0.557
6	10.127	25475	2391	0.187
7	10.274	44876	2374	0.329
Total		13645272	596145	100.000