

Sample Name : Melittin,honey bee
 Cat. No. :RP20415
 Lot. No. :E4971019I
 Time Processed :14:16:23
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
31.00	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

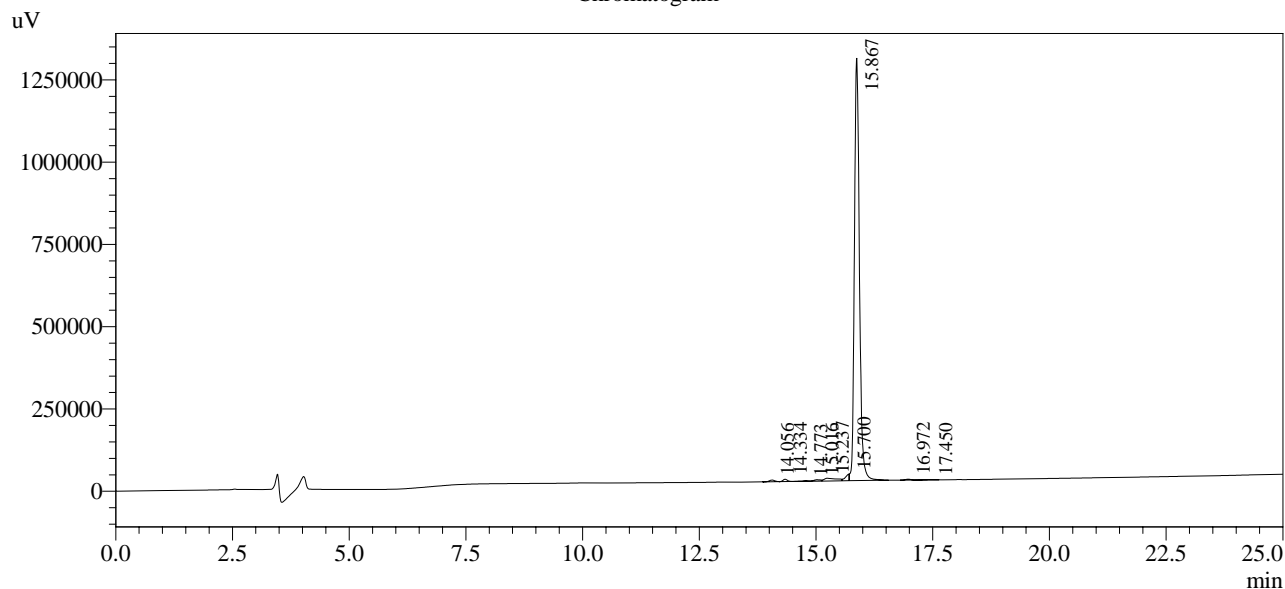

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.056	41586	5186	0.411
2	14.334	46469	7124	0.459
3	14.773	18947	1907	0.187
4	15.016	46336	4276	0.458
5	15.237	159803	8553	1.580
6	15.700	111940	19978	1.106
7	15.867	9656972	1283356	95.456
8	16.972	24243	2981	0.240
9	17.450	10367	806	0.102
Total		10116663	1334166	100.000