

Sample Name:RGD

Cat.No.:RP20297 Lot.No.:PE7241711

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min


Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
30.01	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

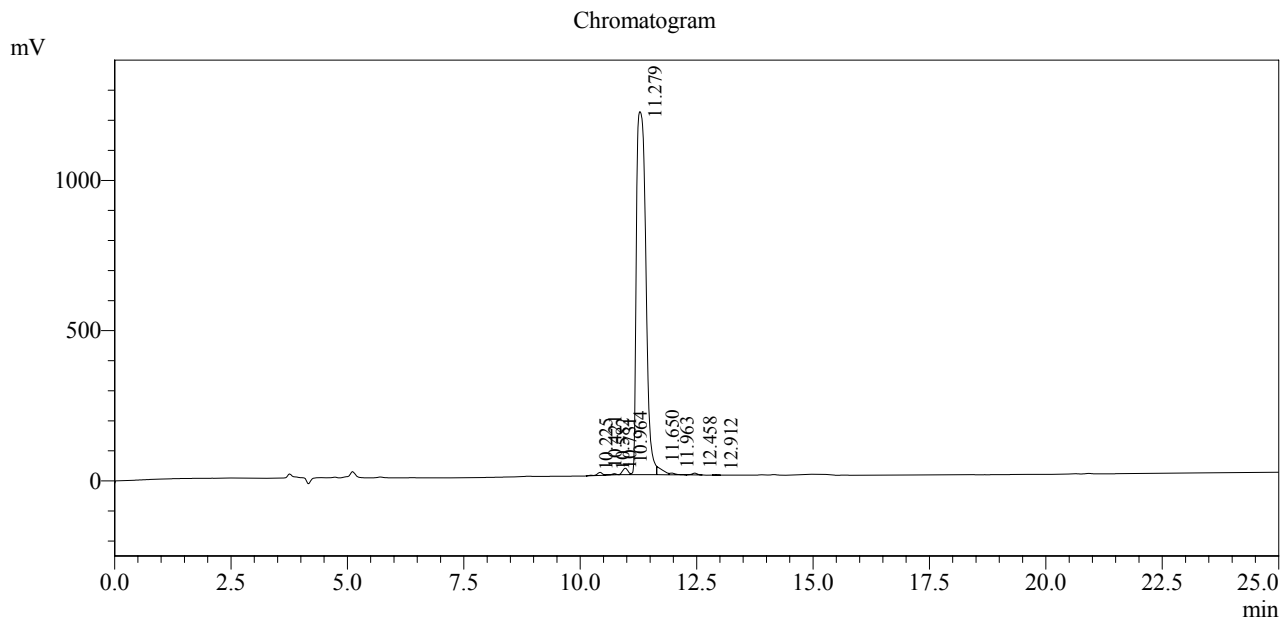

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.225	11104	1565	0.063
2	10.421	70278	10118	0.399
3	10.582	11039	1704	0.063
4	10.731	21583	3585	0.123
5	10.964	170678	21349	0.969
6	11.279	16996305	1208290	96.539
7	11.650	228593	26949	1.298
8	11.963	48415	5508	0.275
9	12.458	44007	5816	0.250
10	12.912	3725	659	0.021
Total		17605727	1285542	100.000