

Sample Name :Substance P
 Cat No. :RP10178
 Lot No. :E9488820B
 Time Processed :8:45:10
 Month-Day-Year Processed :02/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

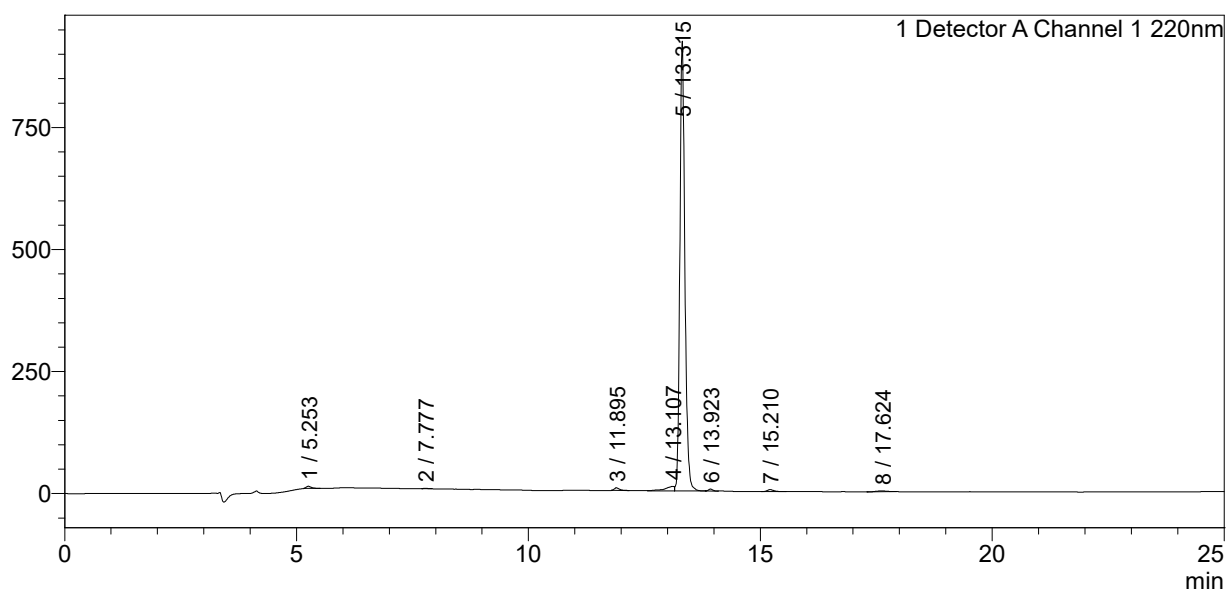

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.253	35475	4560	0.489
2	7.777	5819	982	0.080
3	11.895	41358	5339	0.570
4	13.107	133263	9419	1.838
5	13.315	6940460	921795	95.715
6	13.923	27945	4159	0.385
7	15.210	38401	3985	0.530
8	17.624	28440	1703	0.392
Total		7251161	951943	100.000