

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide
 Cat No. : RP21087
 Lot No. : E80033201
 Time Processed :1:01:47
 Month-Day-Year Processed :10/01/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

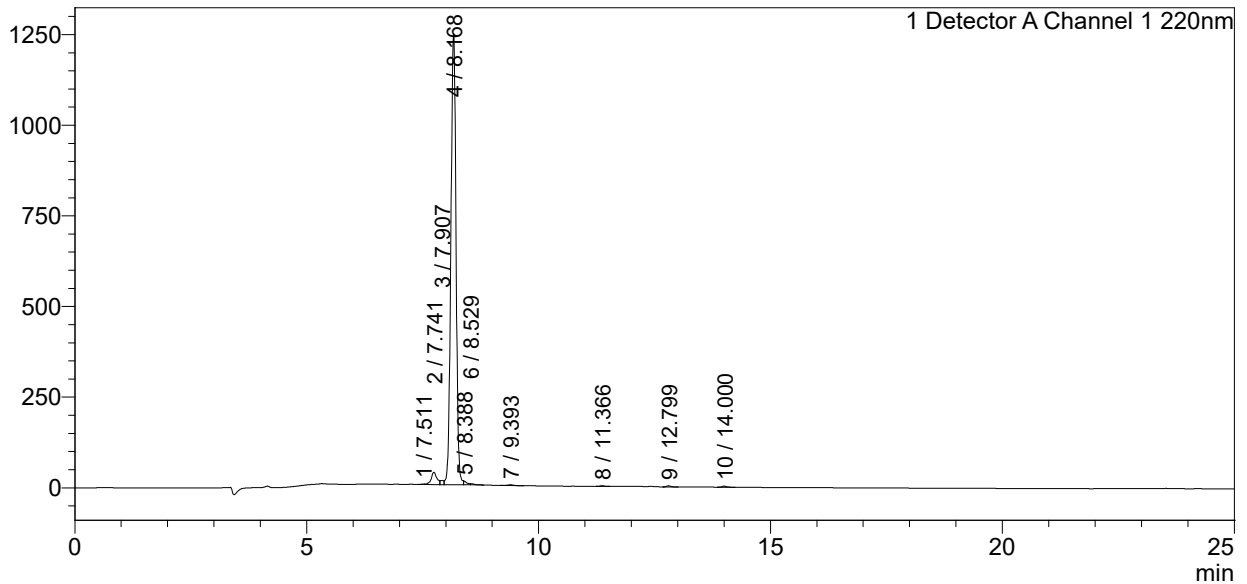

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.511	5866	1221	0.058
2	7.741	298608	34252	2.966
3	7.907	55929	11506	0.556
4	8.168	9566275	1244597	95.031
5	8.388	50734	10779	0.504
6	8.529	20361	3397	0.202
7	9.393	17433	1879	0.173
8	11.366	12014	2224	0.119
9	12.799	18940	3137	0.188
10	14.000	20338	2880	0.202
Total		10066497	1315870	100.000