

Sample Name :OVA Peptide (257-264)  
 Cat No.: RP10611  
 Lot No.: E1643019K  
 Time Processed:8:25:52  
 Month-Day-Year Processed:11/15/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

<Chromatogram>

mV

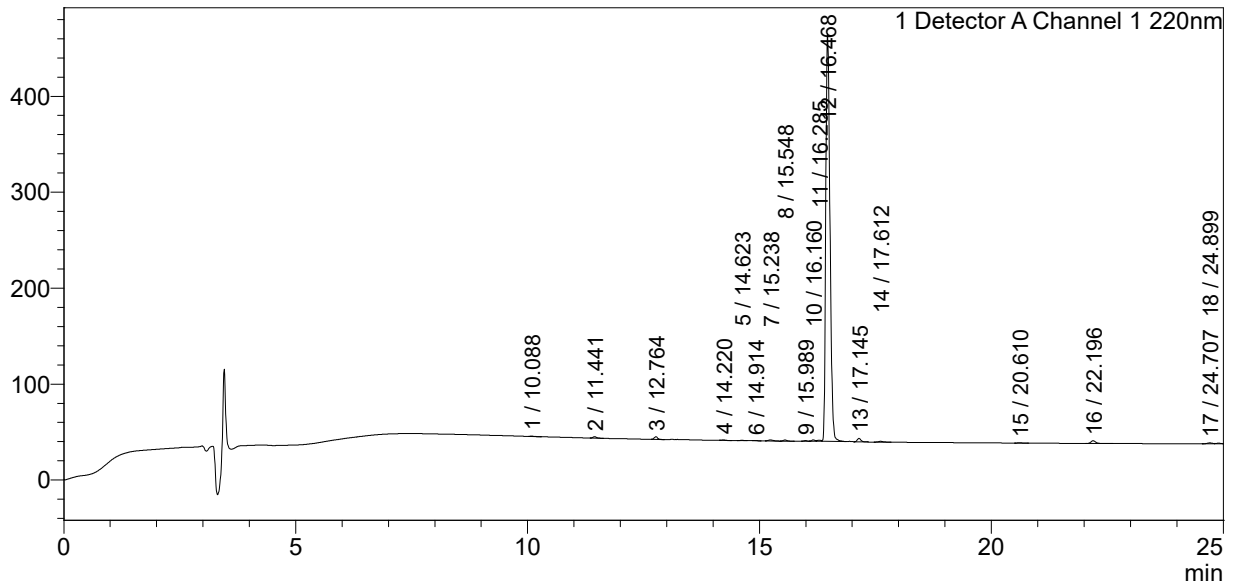

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.088	1763	367	0.063
2	11.441	8173	1555	0.291
3	12.764	13886	2778	0.494
4	14.220	2867	576	0.102
5	14.623	2080	394	0.074
6	14.914	1466	340	0.052
7	15.238	7718	1024	0.274
8	15.548	6727	1151	0.239
9	15.989	2954	662	0.105
10	16.160	7713	1459	0.274
11	16.285	7353	1195	0.261
12	16.468	2689995	425083	95.670
13	17.145	19334	3485	0.688
14	17.612	5812	820	0.207
15	20.610	2118	358	0.075

Peak#	Ret. Time	Area	Height	Area%
16	22.196	20466	2839	0.728
17	24.707	7299	903	0.260
18	24.899	4021	590	0.143
Total		2811745	445576	100.000