


Mass Spectrum

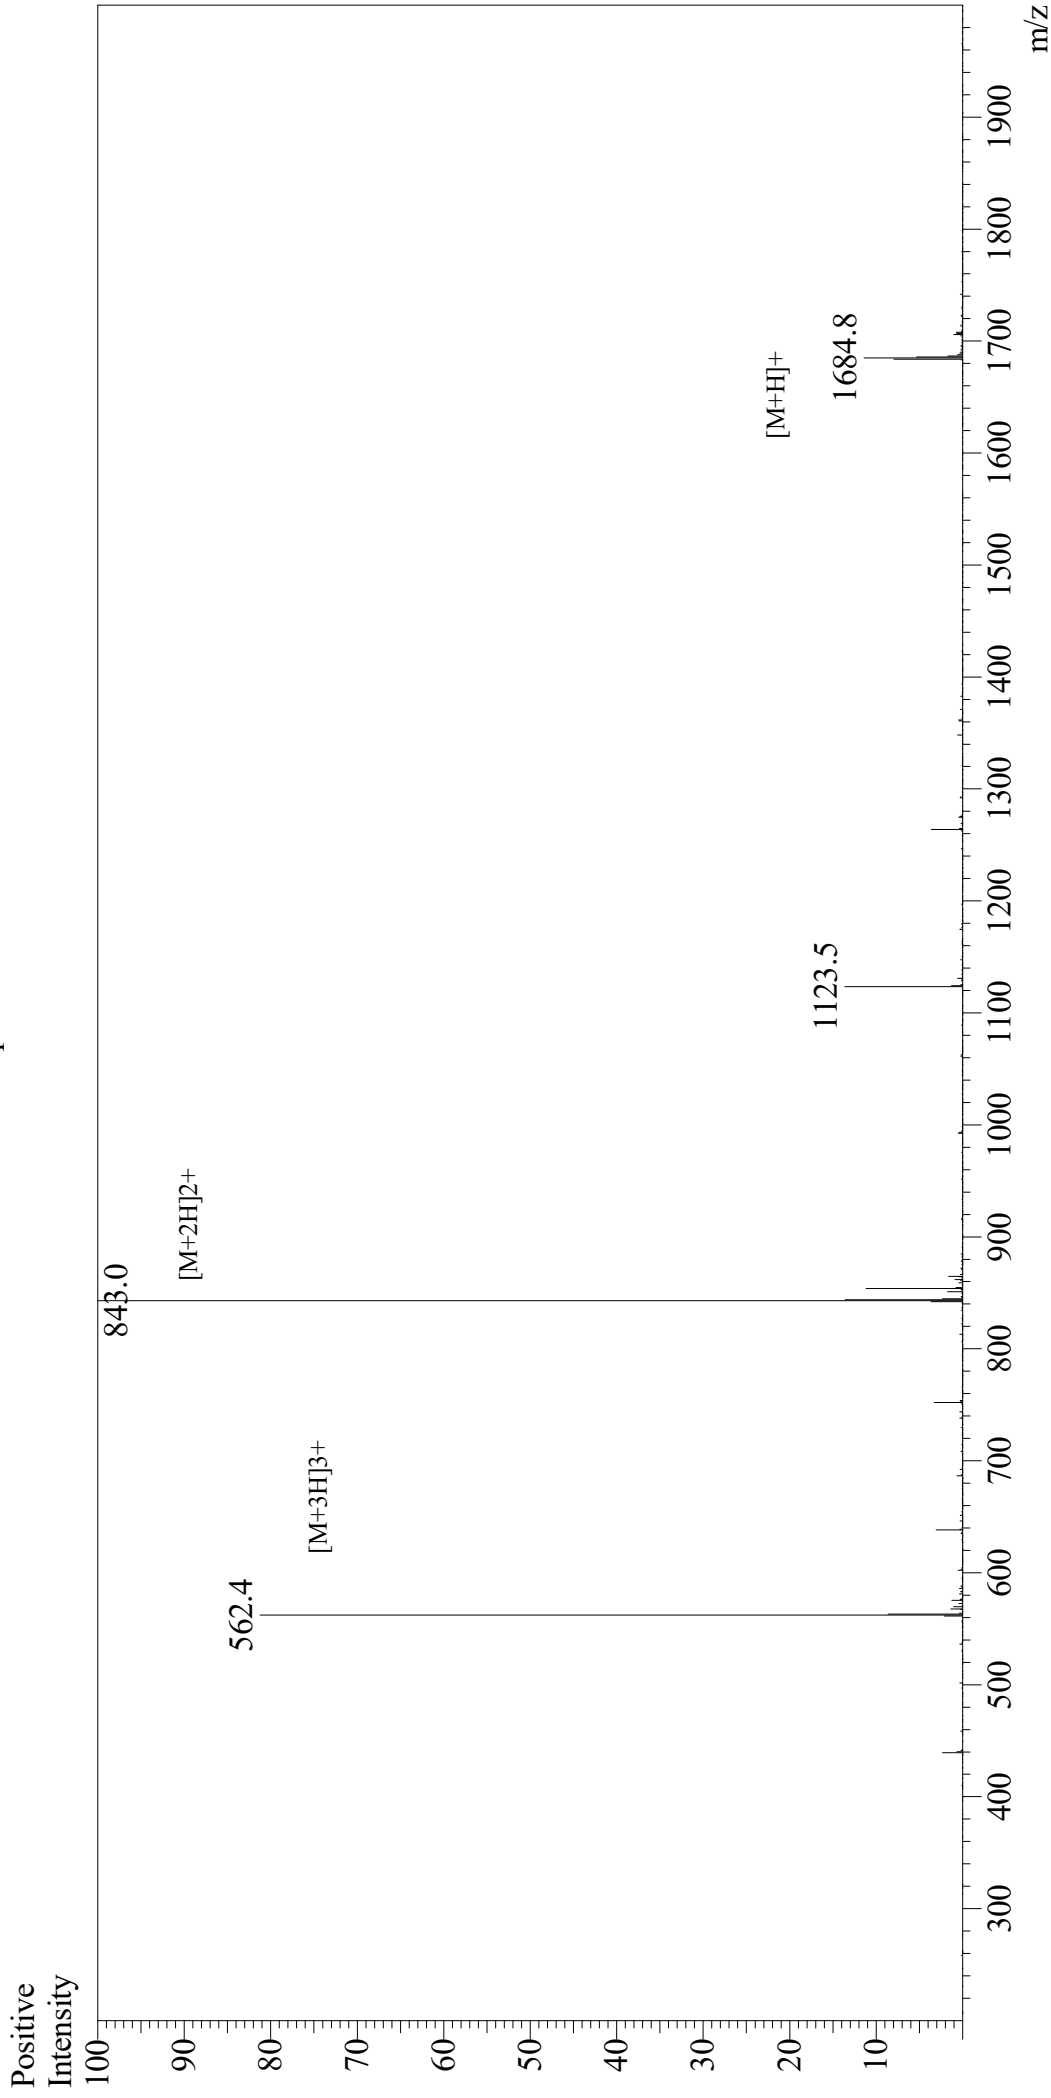

Sample Information

User : Gary
Month-Day Processed : 01/23/19
Time Processed : 04:58:45 PM
Injection Volume : 0.2
Sample Name : α -Factor Mating Pheromone, yeast
Cat No. : RP01002
Lot No. : PE6141901
Theoretical MW : 1683.98
Observed MW : 1684.0

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200