

Sample Name :c-Myc Peptide
 Cat No. :RP11731
 Lot No. :E8191221C
 Time Processed :10:45:09 AM
 Month-Day-Year Processed :03/15/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

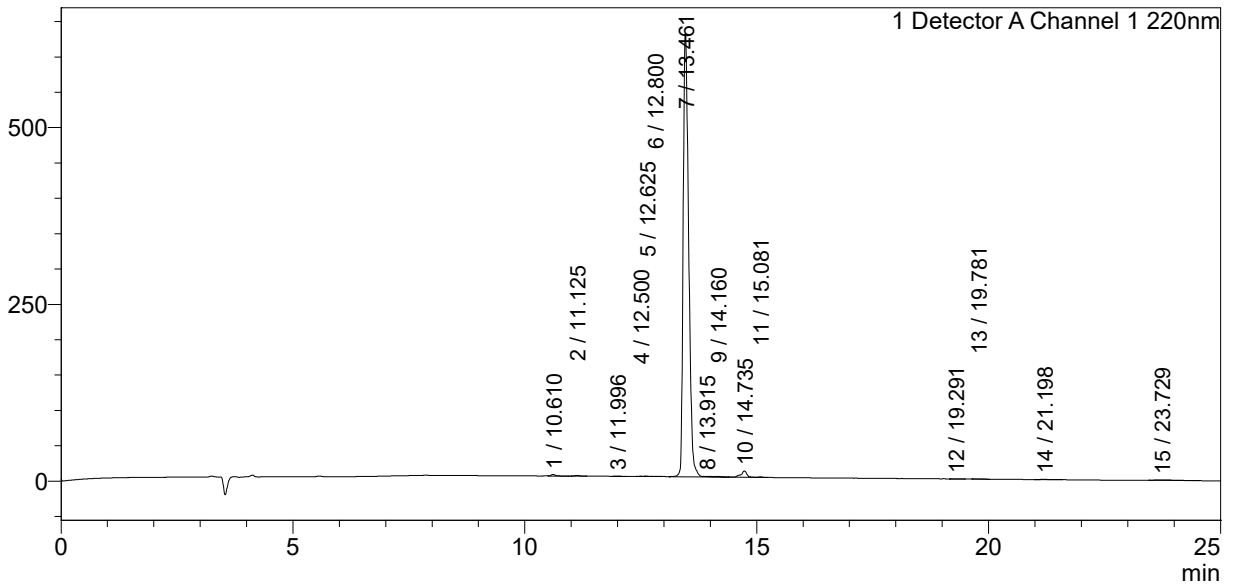

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.610	14677	2204	0.275
2	11.125	6907	947	0.129
3	11.996	3574	488	0.067
4	12.500	1448	217	0.027
5	12.625	2274	437	0.043
6	12.800	1481	260	0.028
7	13.461	5180880	626889	97.031
8	13.915	2515	468	0.047
9	14.160	6140	676	0.115
10	14.735	77809	8888	1.457
11	15.081	4376	716	0.082
12	19.291	1131	128	0.021
13	19.781	2907	324	0.054
14	21.198	4521	315	0.085

Peak#	Ret. Time	Area	Height	Area%
15	23.729	28790	860	0.539
Total		5339429	643817	100.000