

Sample Name: β -Amyloid (1-42), human
 Cat No. : RP10017
 Lot No. :E1237720I
 Time Processed: 20:45:21
 Month-Day-Year Processed :11/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|-----------------|-------|
| 0.01 | Pumps | Solvent B Conc. | 10 |
| 25.00 | Pumps | Solvent B Conc. | 100 |
| 25.01 | Pumps | Solvent B Conc. | 95 |
| 27.00 | Pumps | Solvent B Conc. | 95 |
| 27.01 | Pumps | Solvent B Conc. | 10 |
| 35.00 | Pumps | Solvent B Conc. | 10 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

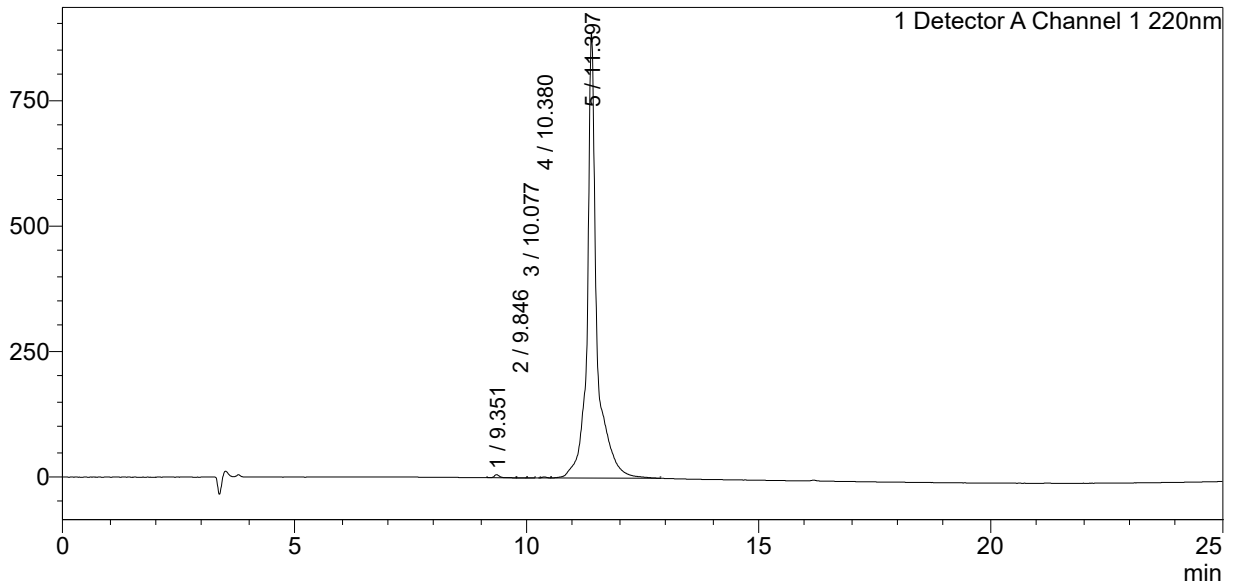

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|--------|---------|
| 1 | 9.351 | 47711 | 6155 | 0.375 |
| 2 | 9.846 | 1542 | 208 | 0.012 |
| 3 | 10.077 | 1392 | 194 | 0.011 |
| 4 | 10.380 | 15351 | 2298 | 0.121 |
| 5 | 11.397 | 12664071 | 884790 | 99.482 |
| Total | | 12730068 | 893646 | 100.000 |